

1/16

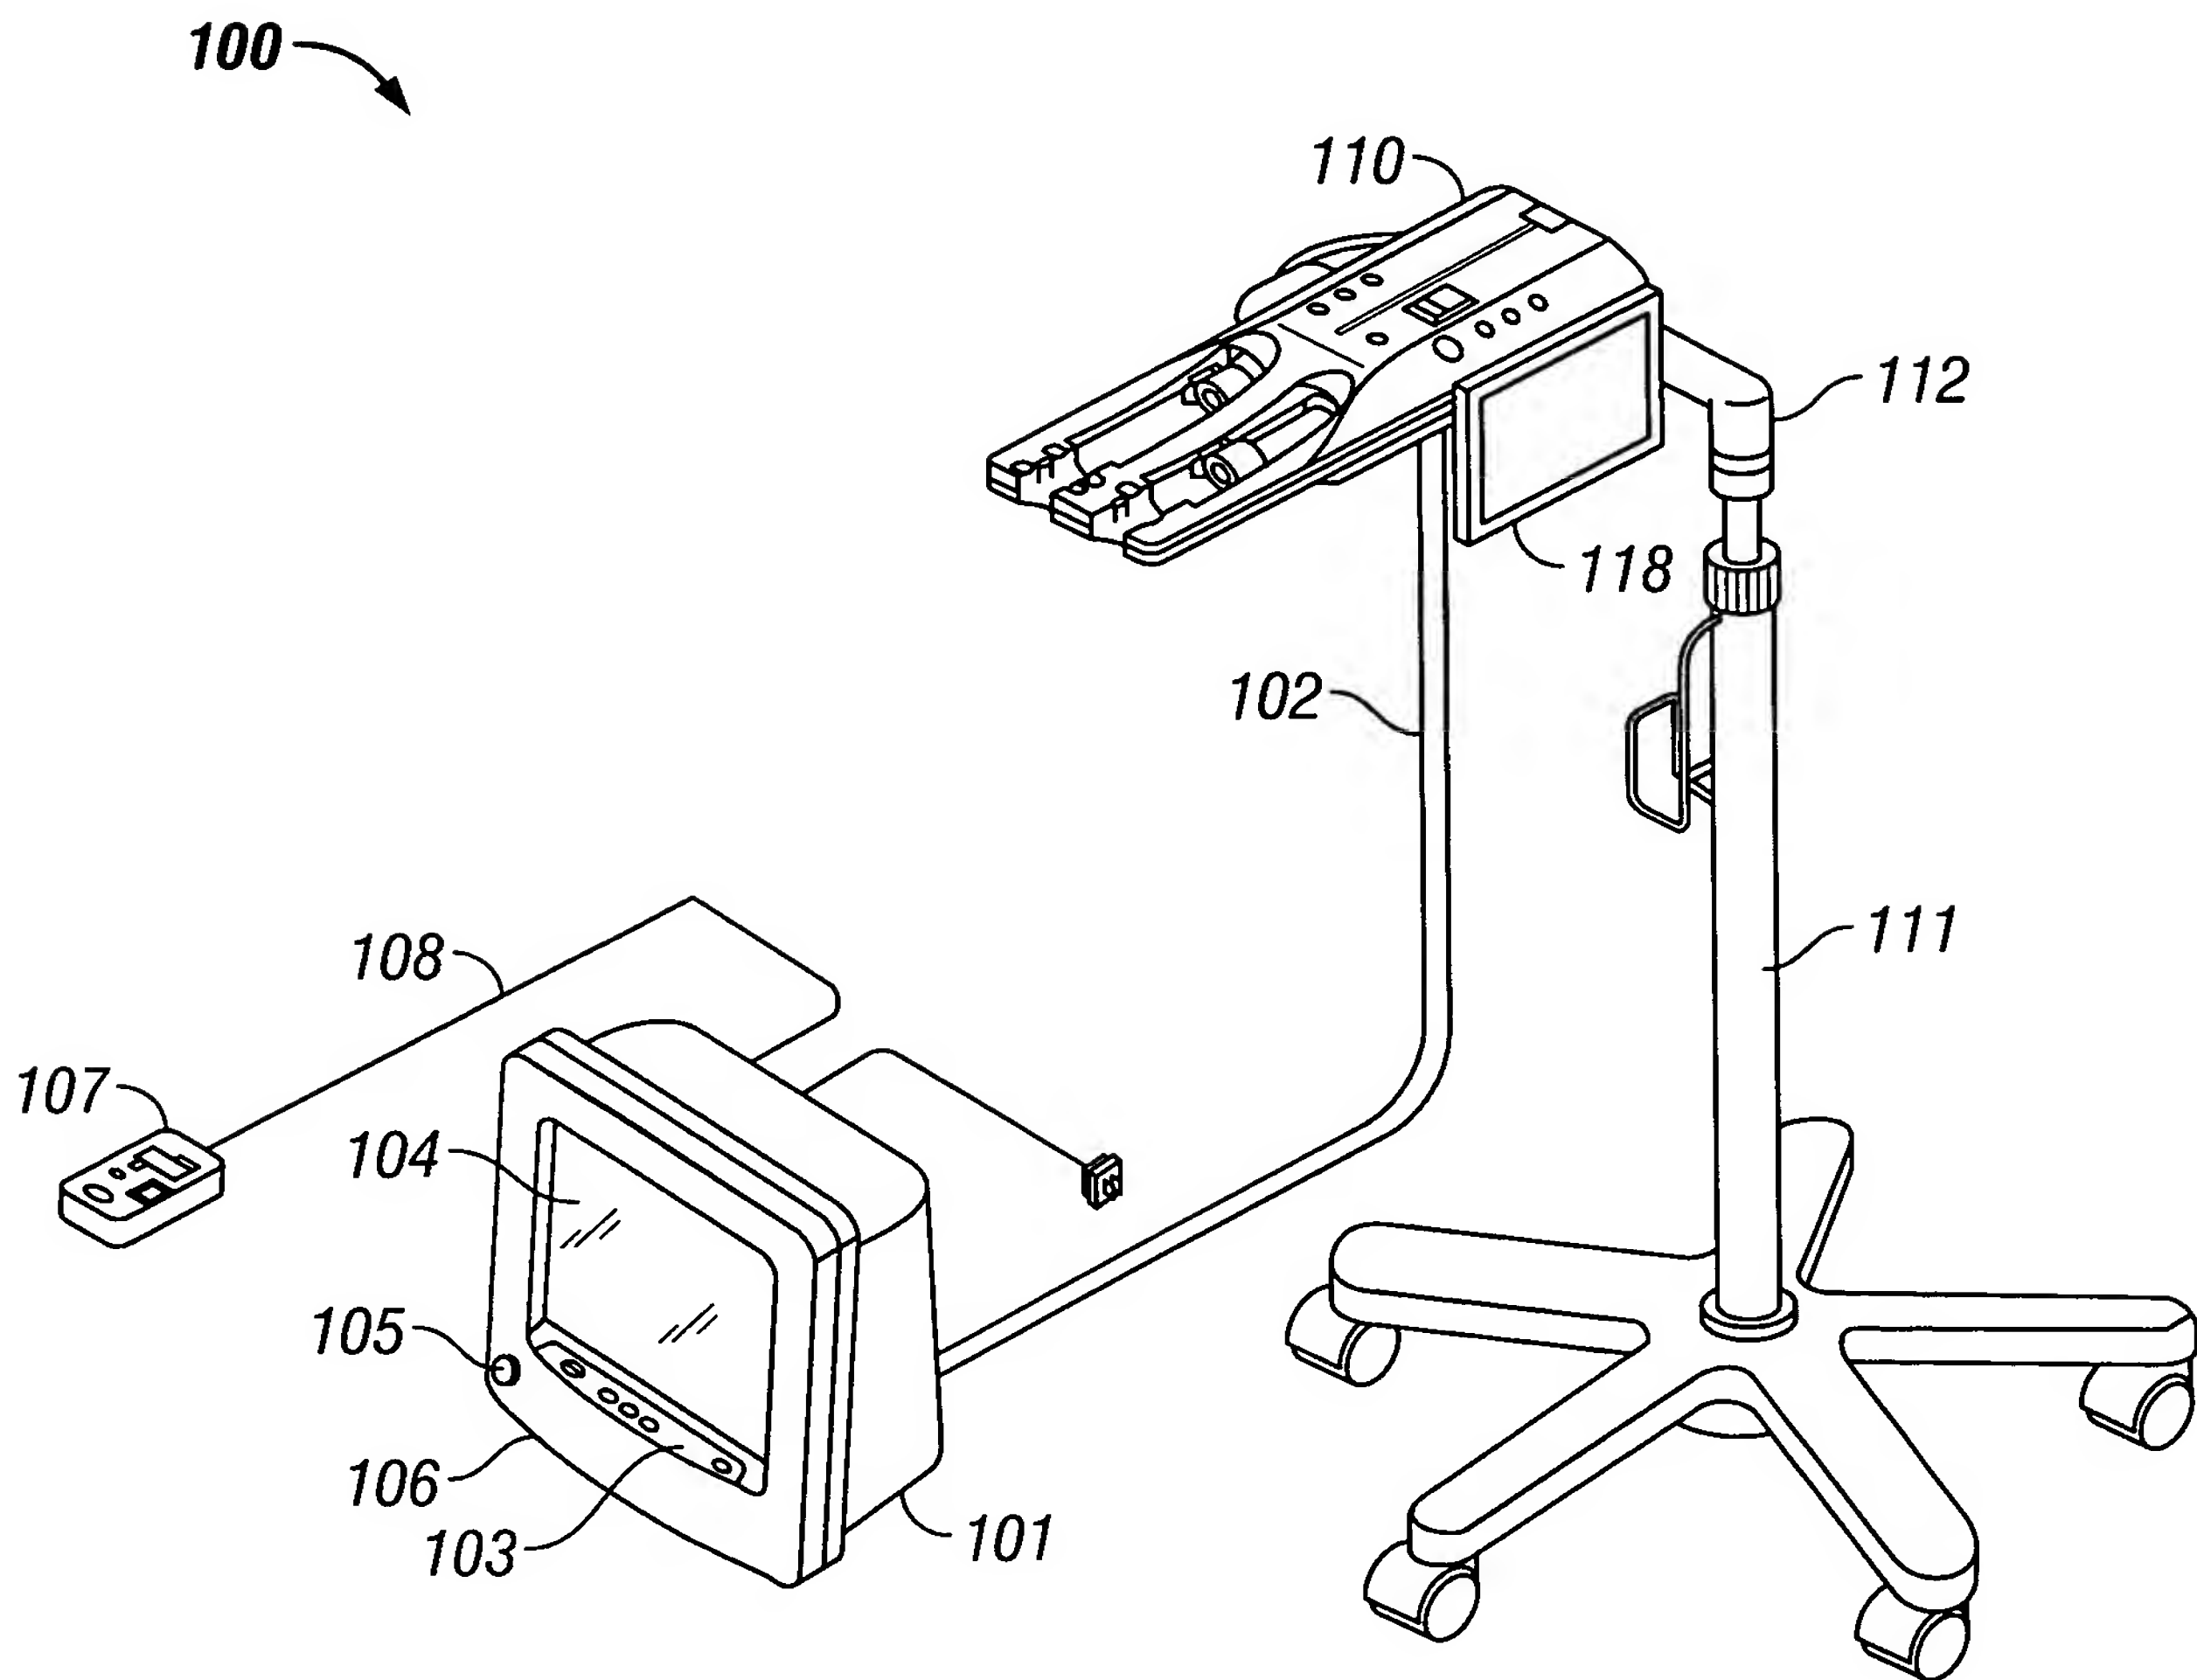


FIG. 1

Nemoto, et al.

Replacement Sheet

2/16

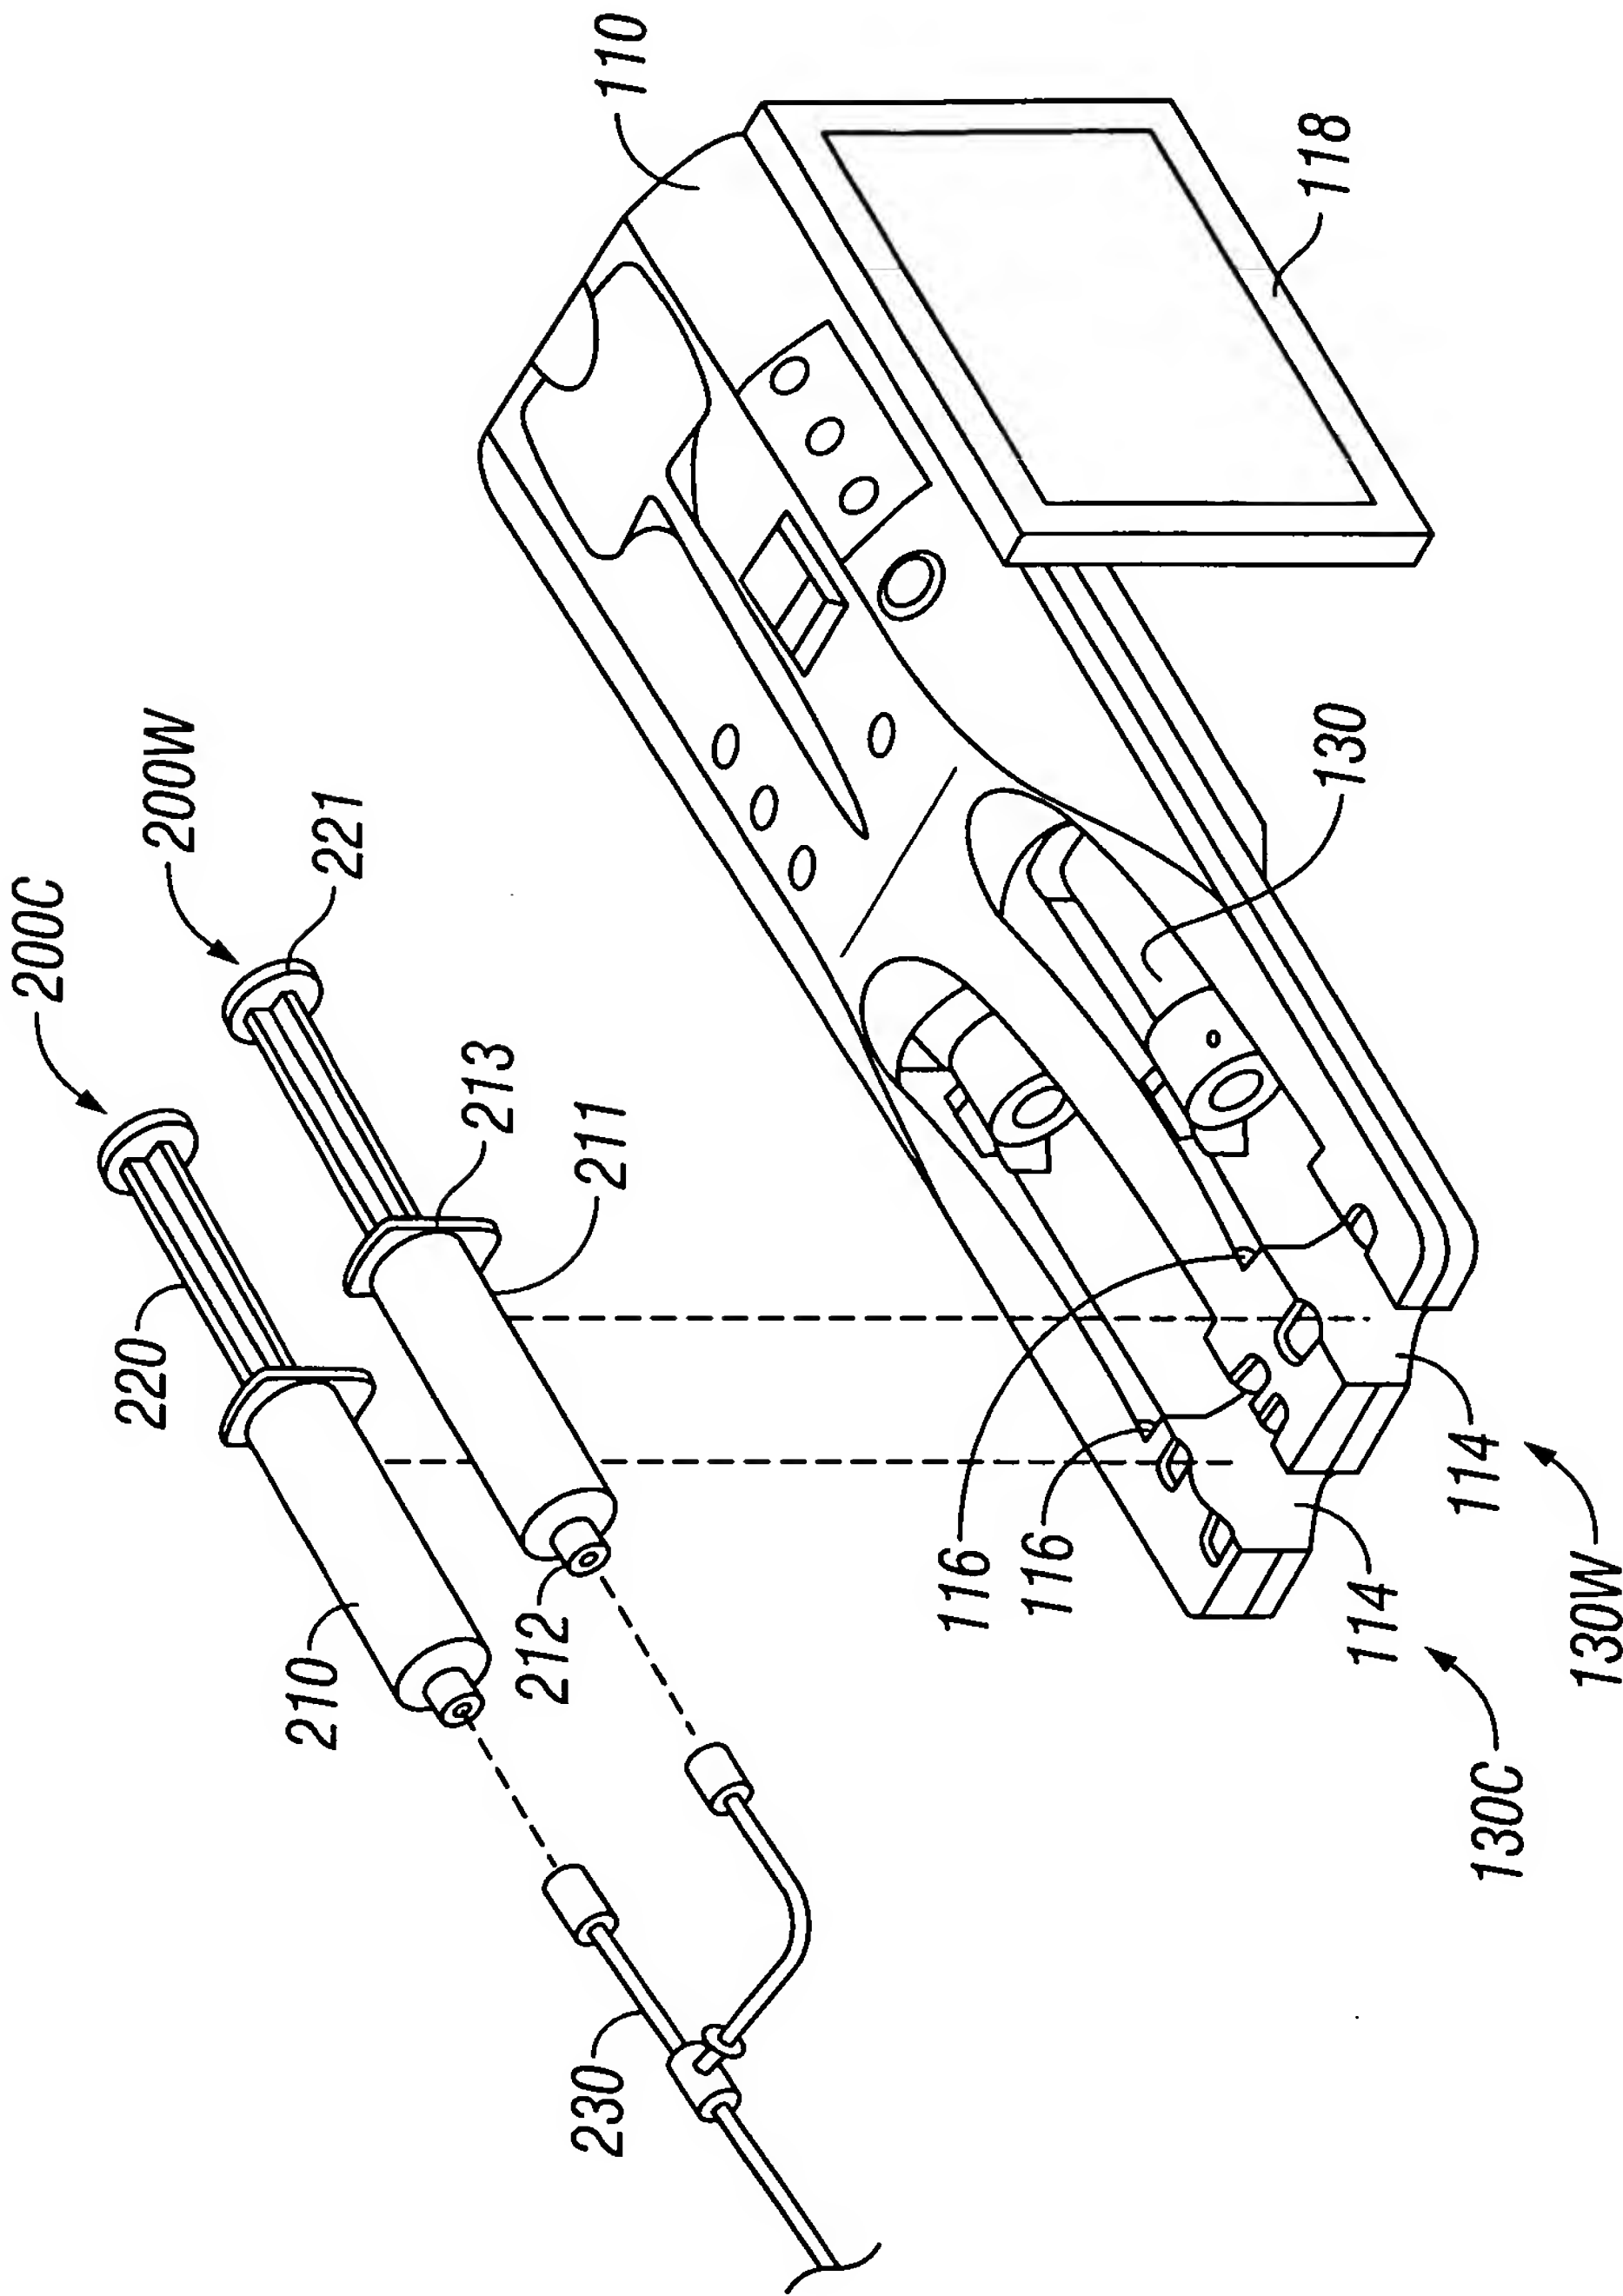


FIG. 2

3/16

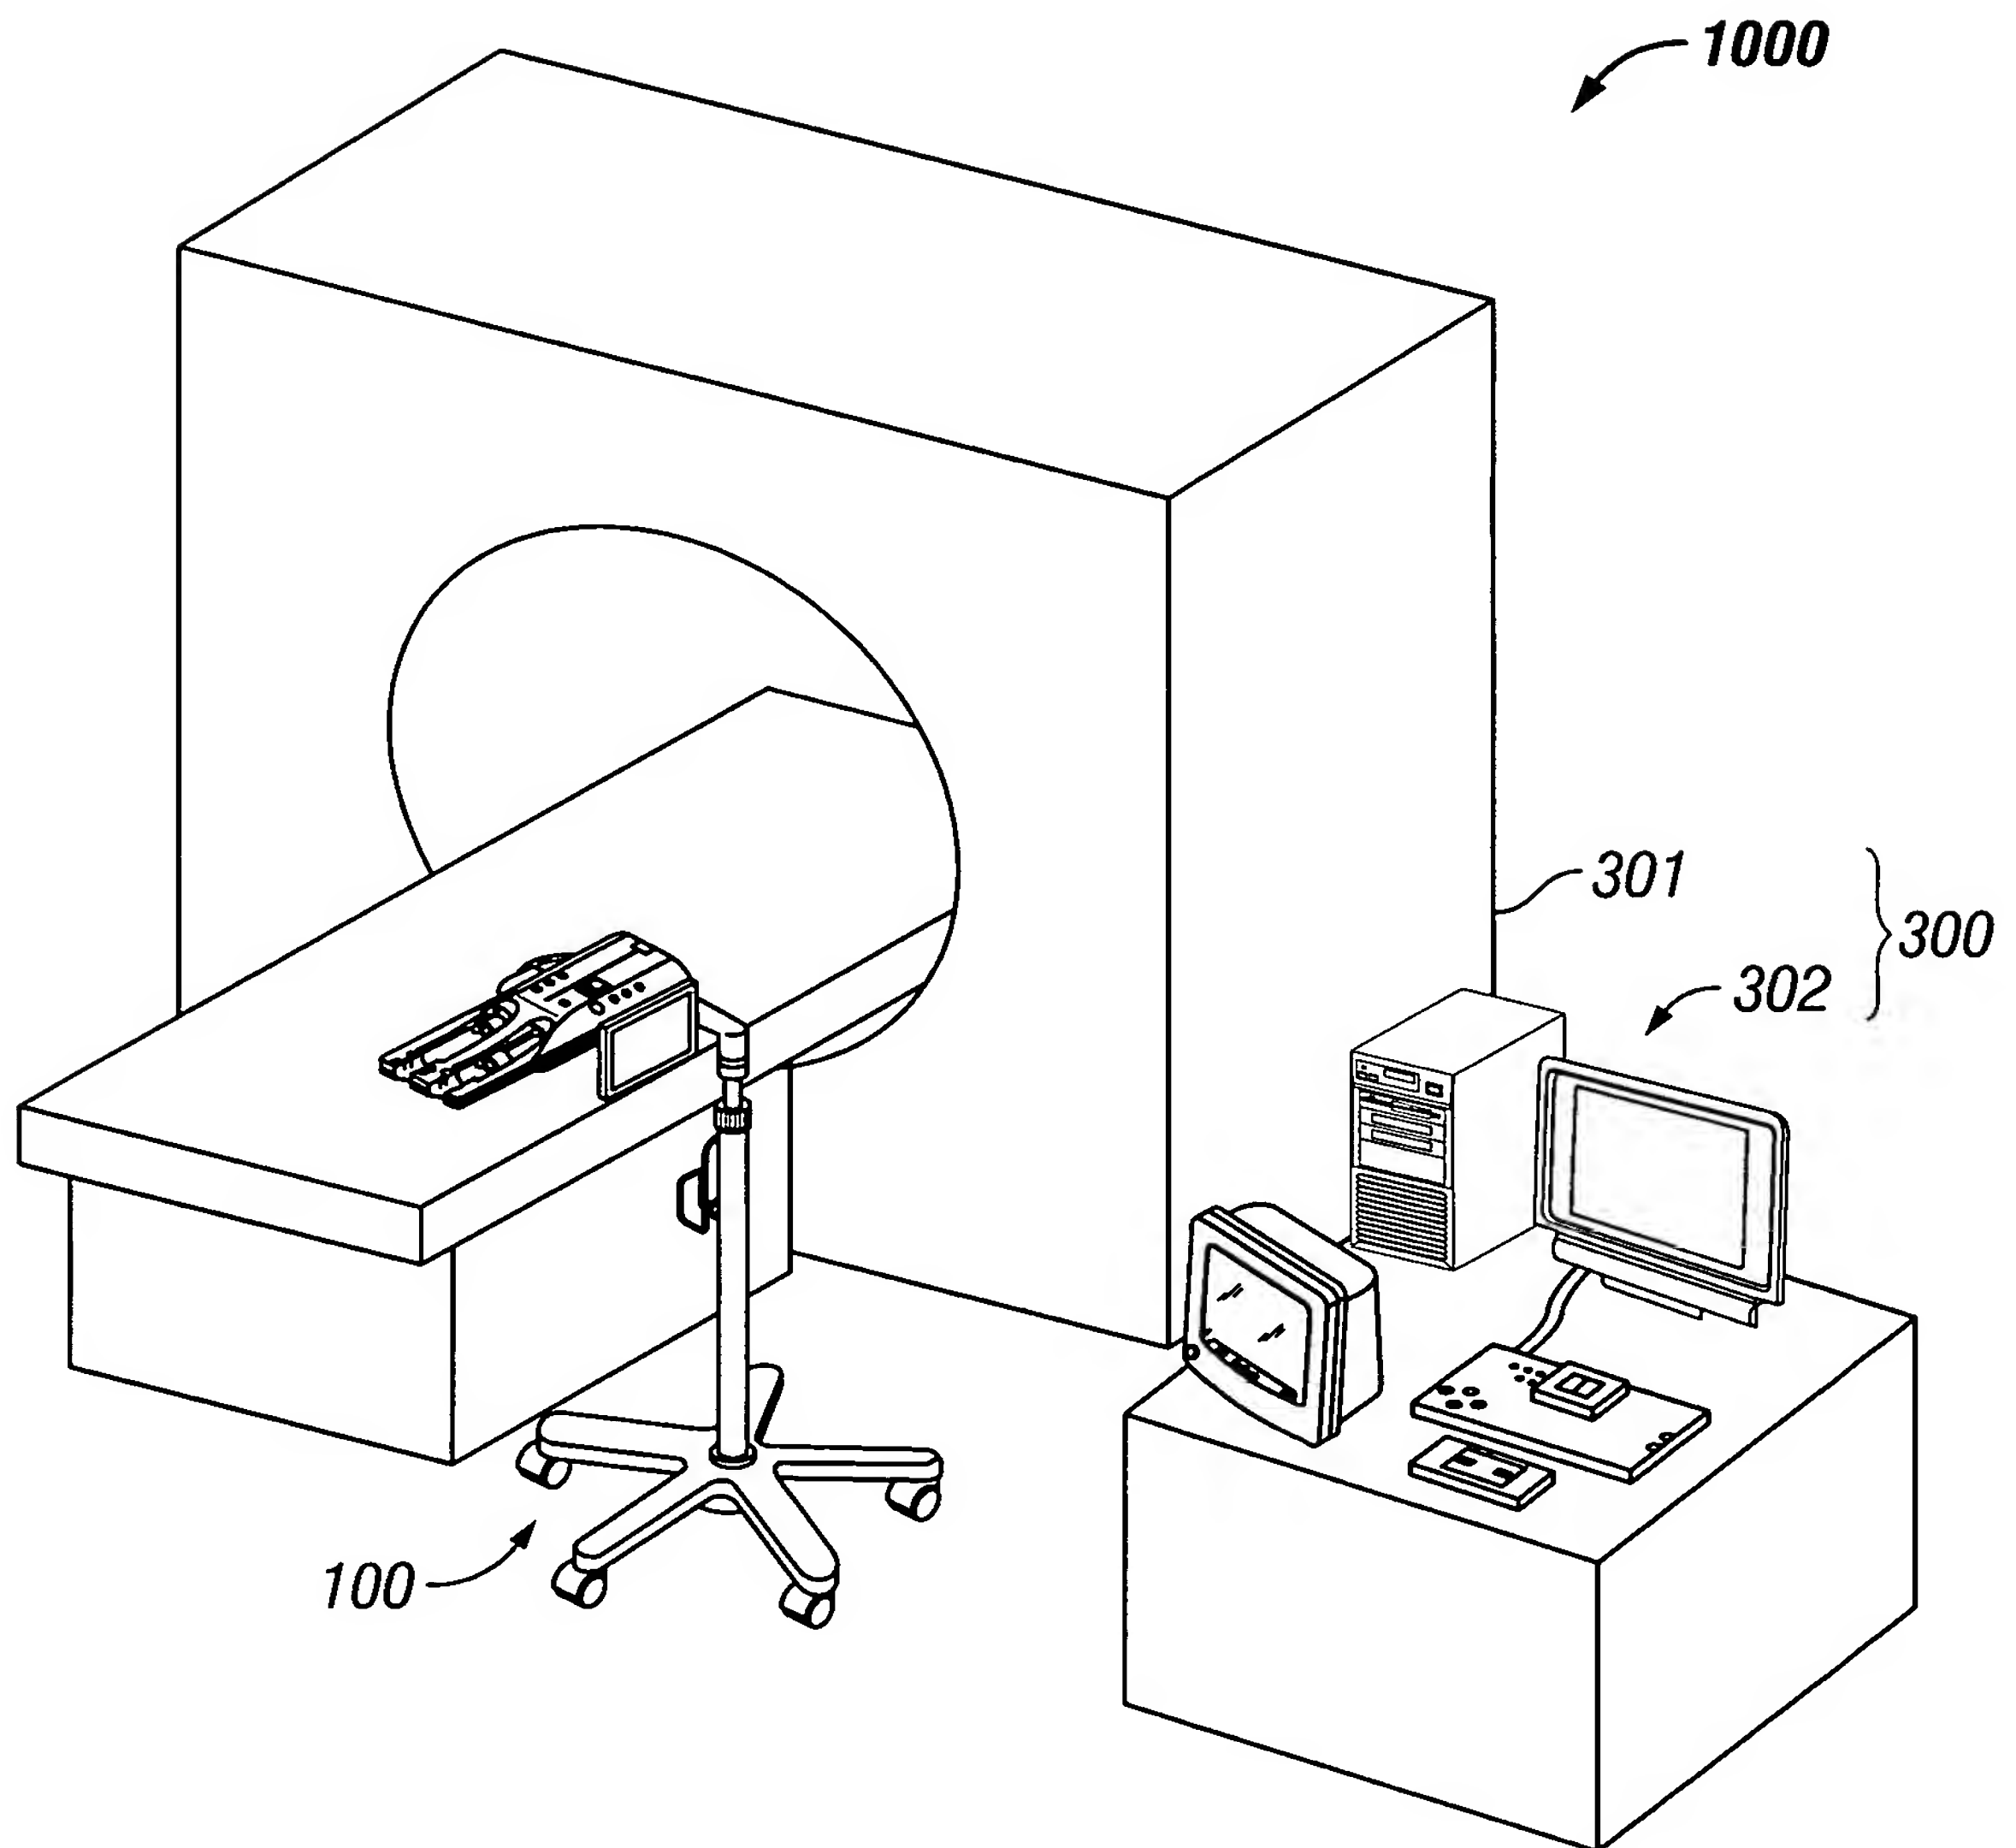


FIG. 3

Nemoto, et al.
 Appl. No.: Unknown Atty Docket: KITO10.001APC
 Replacement Sheet

Replacement Sheet

4/16

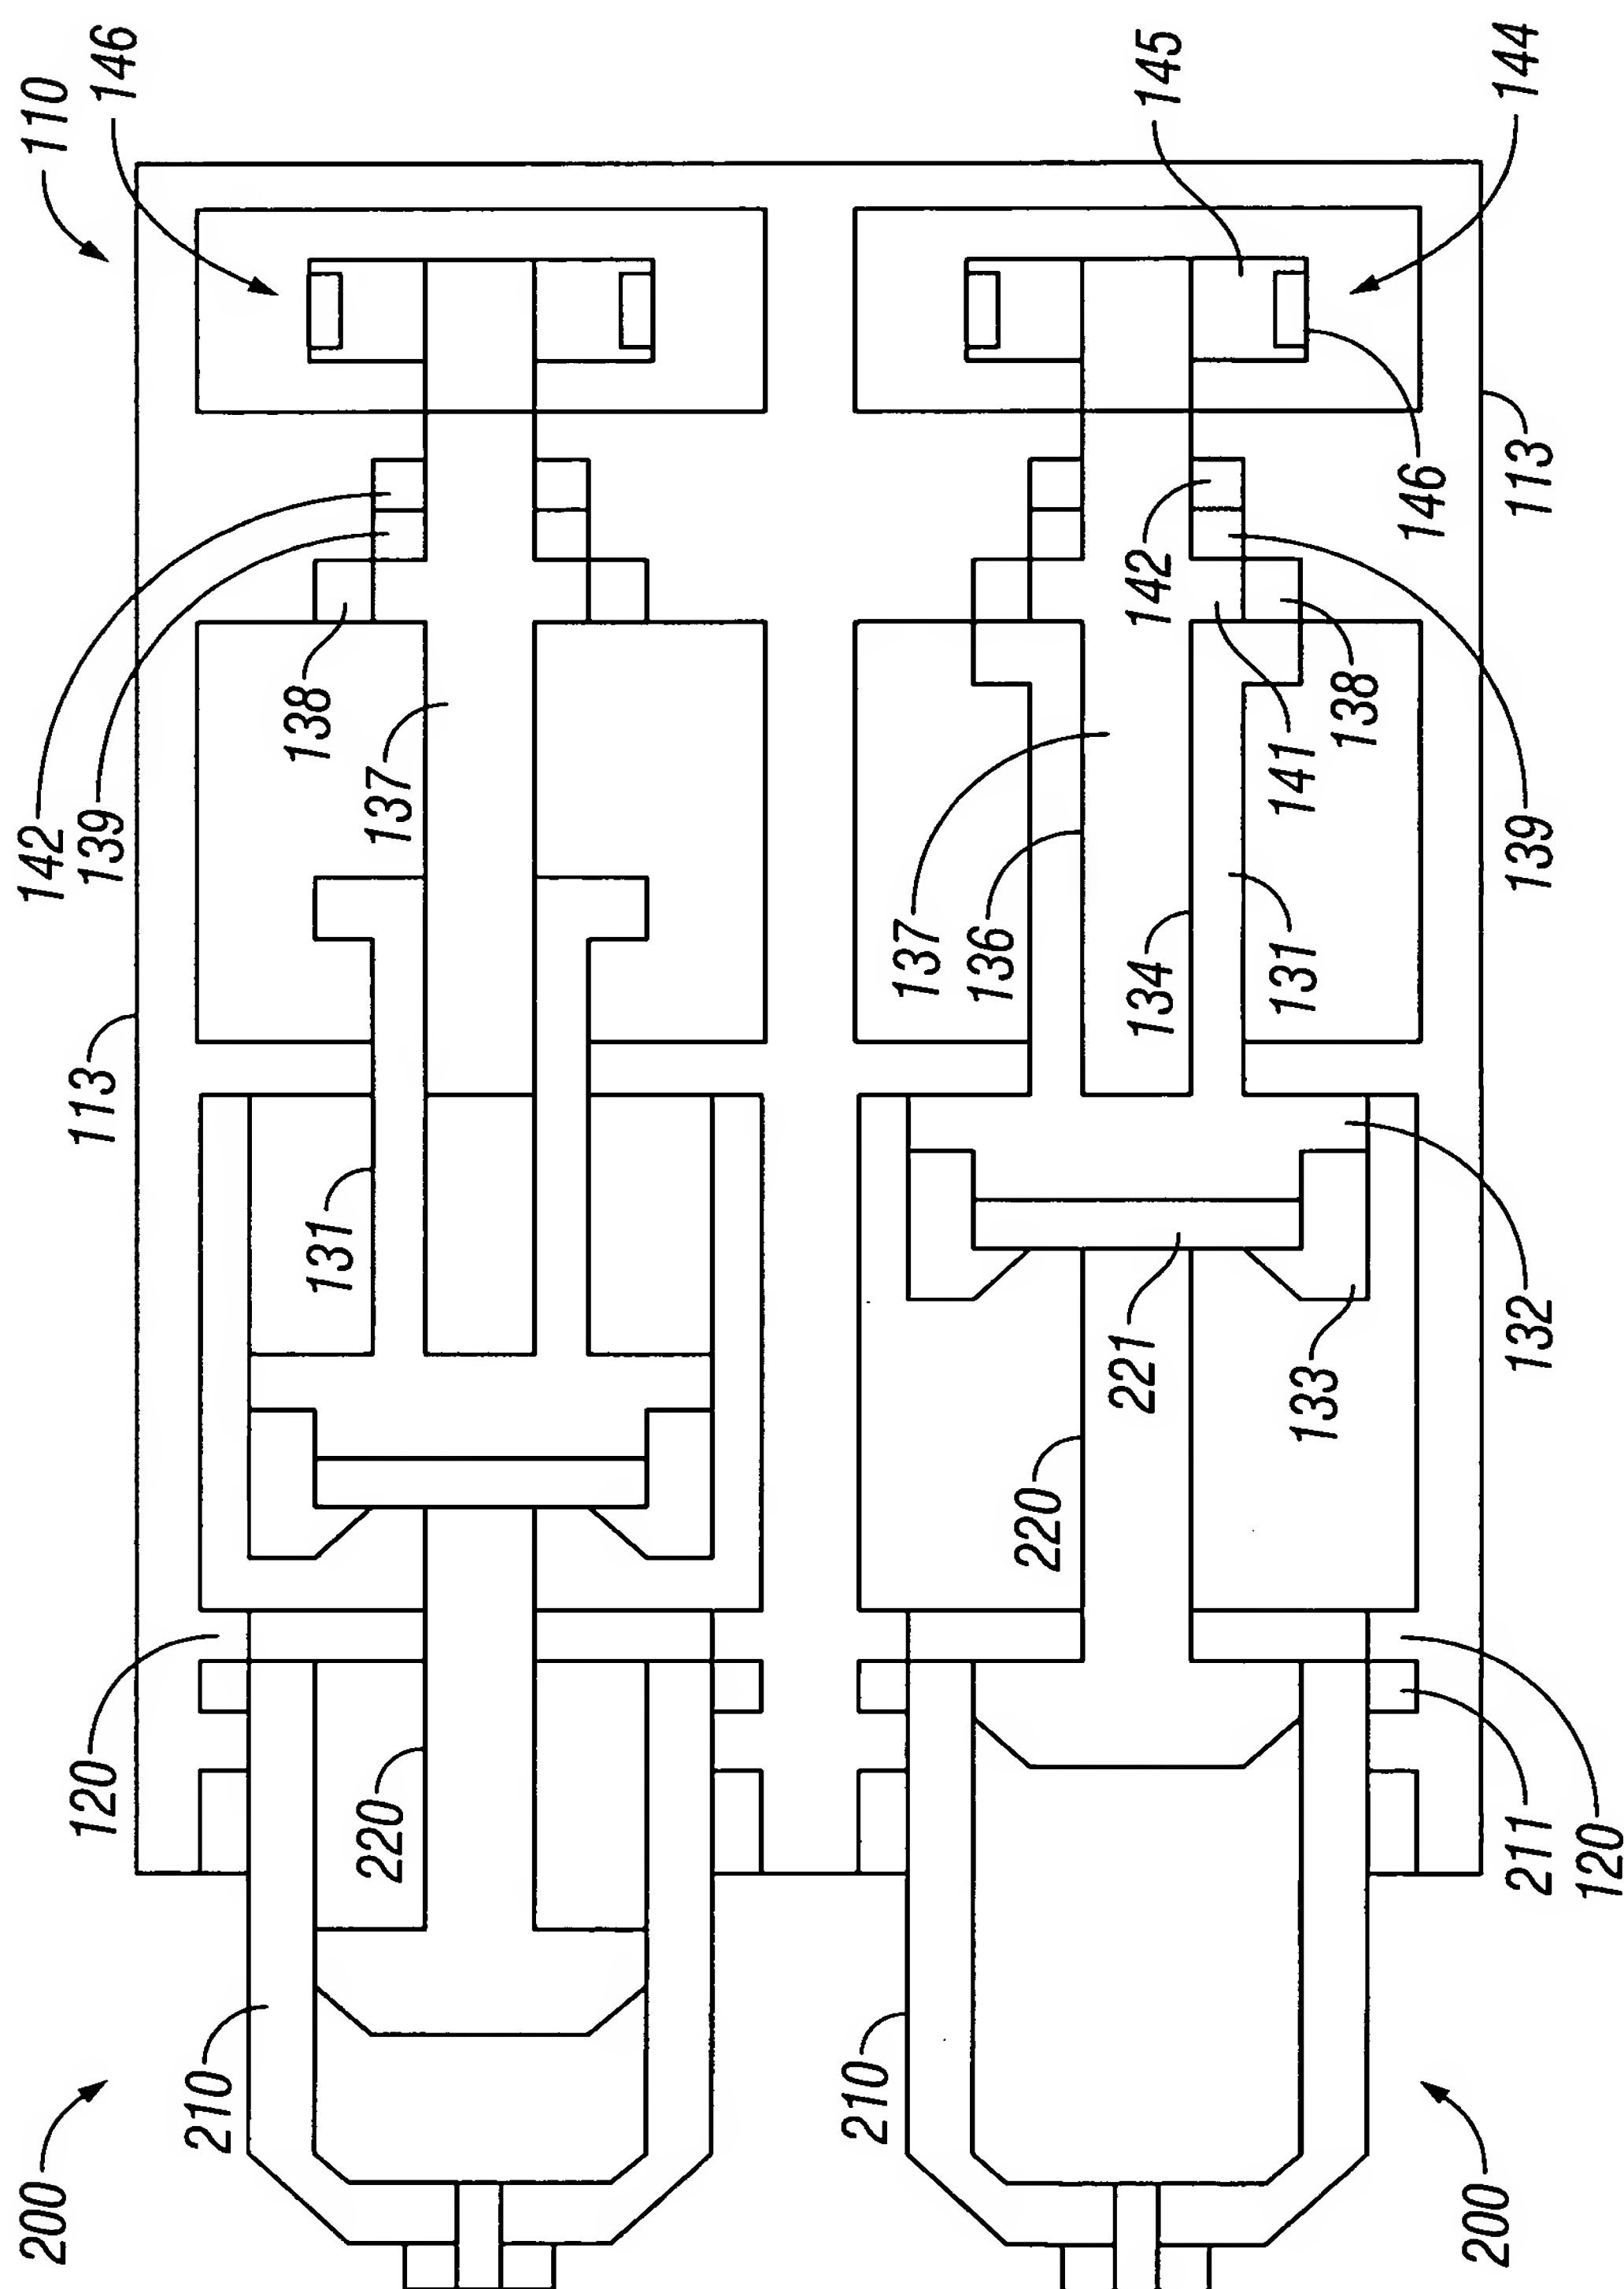


FIG. 4

5/16

1000

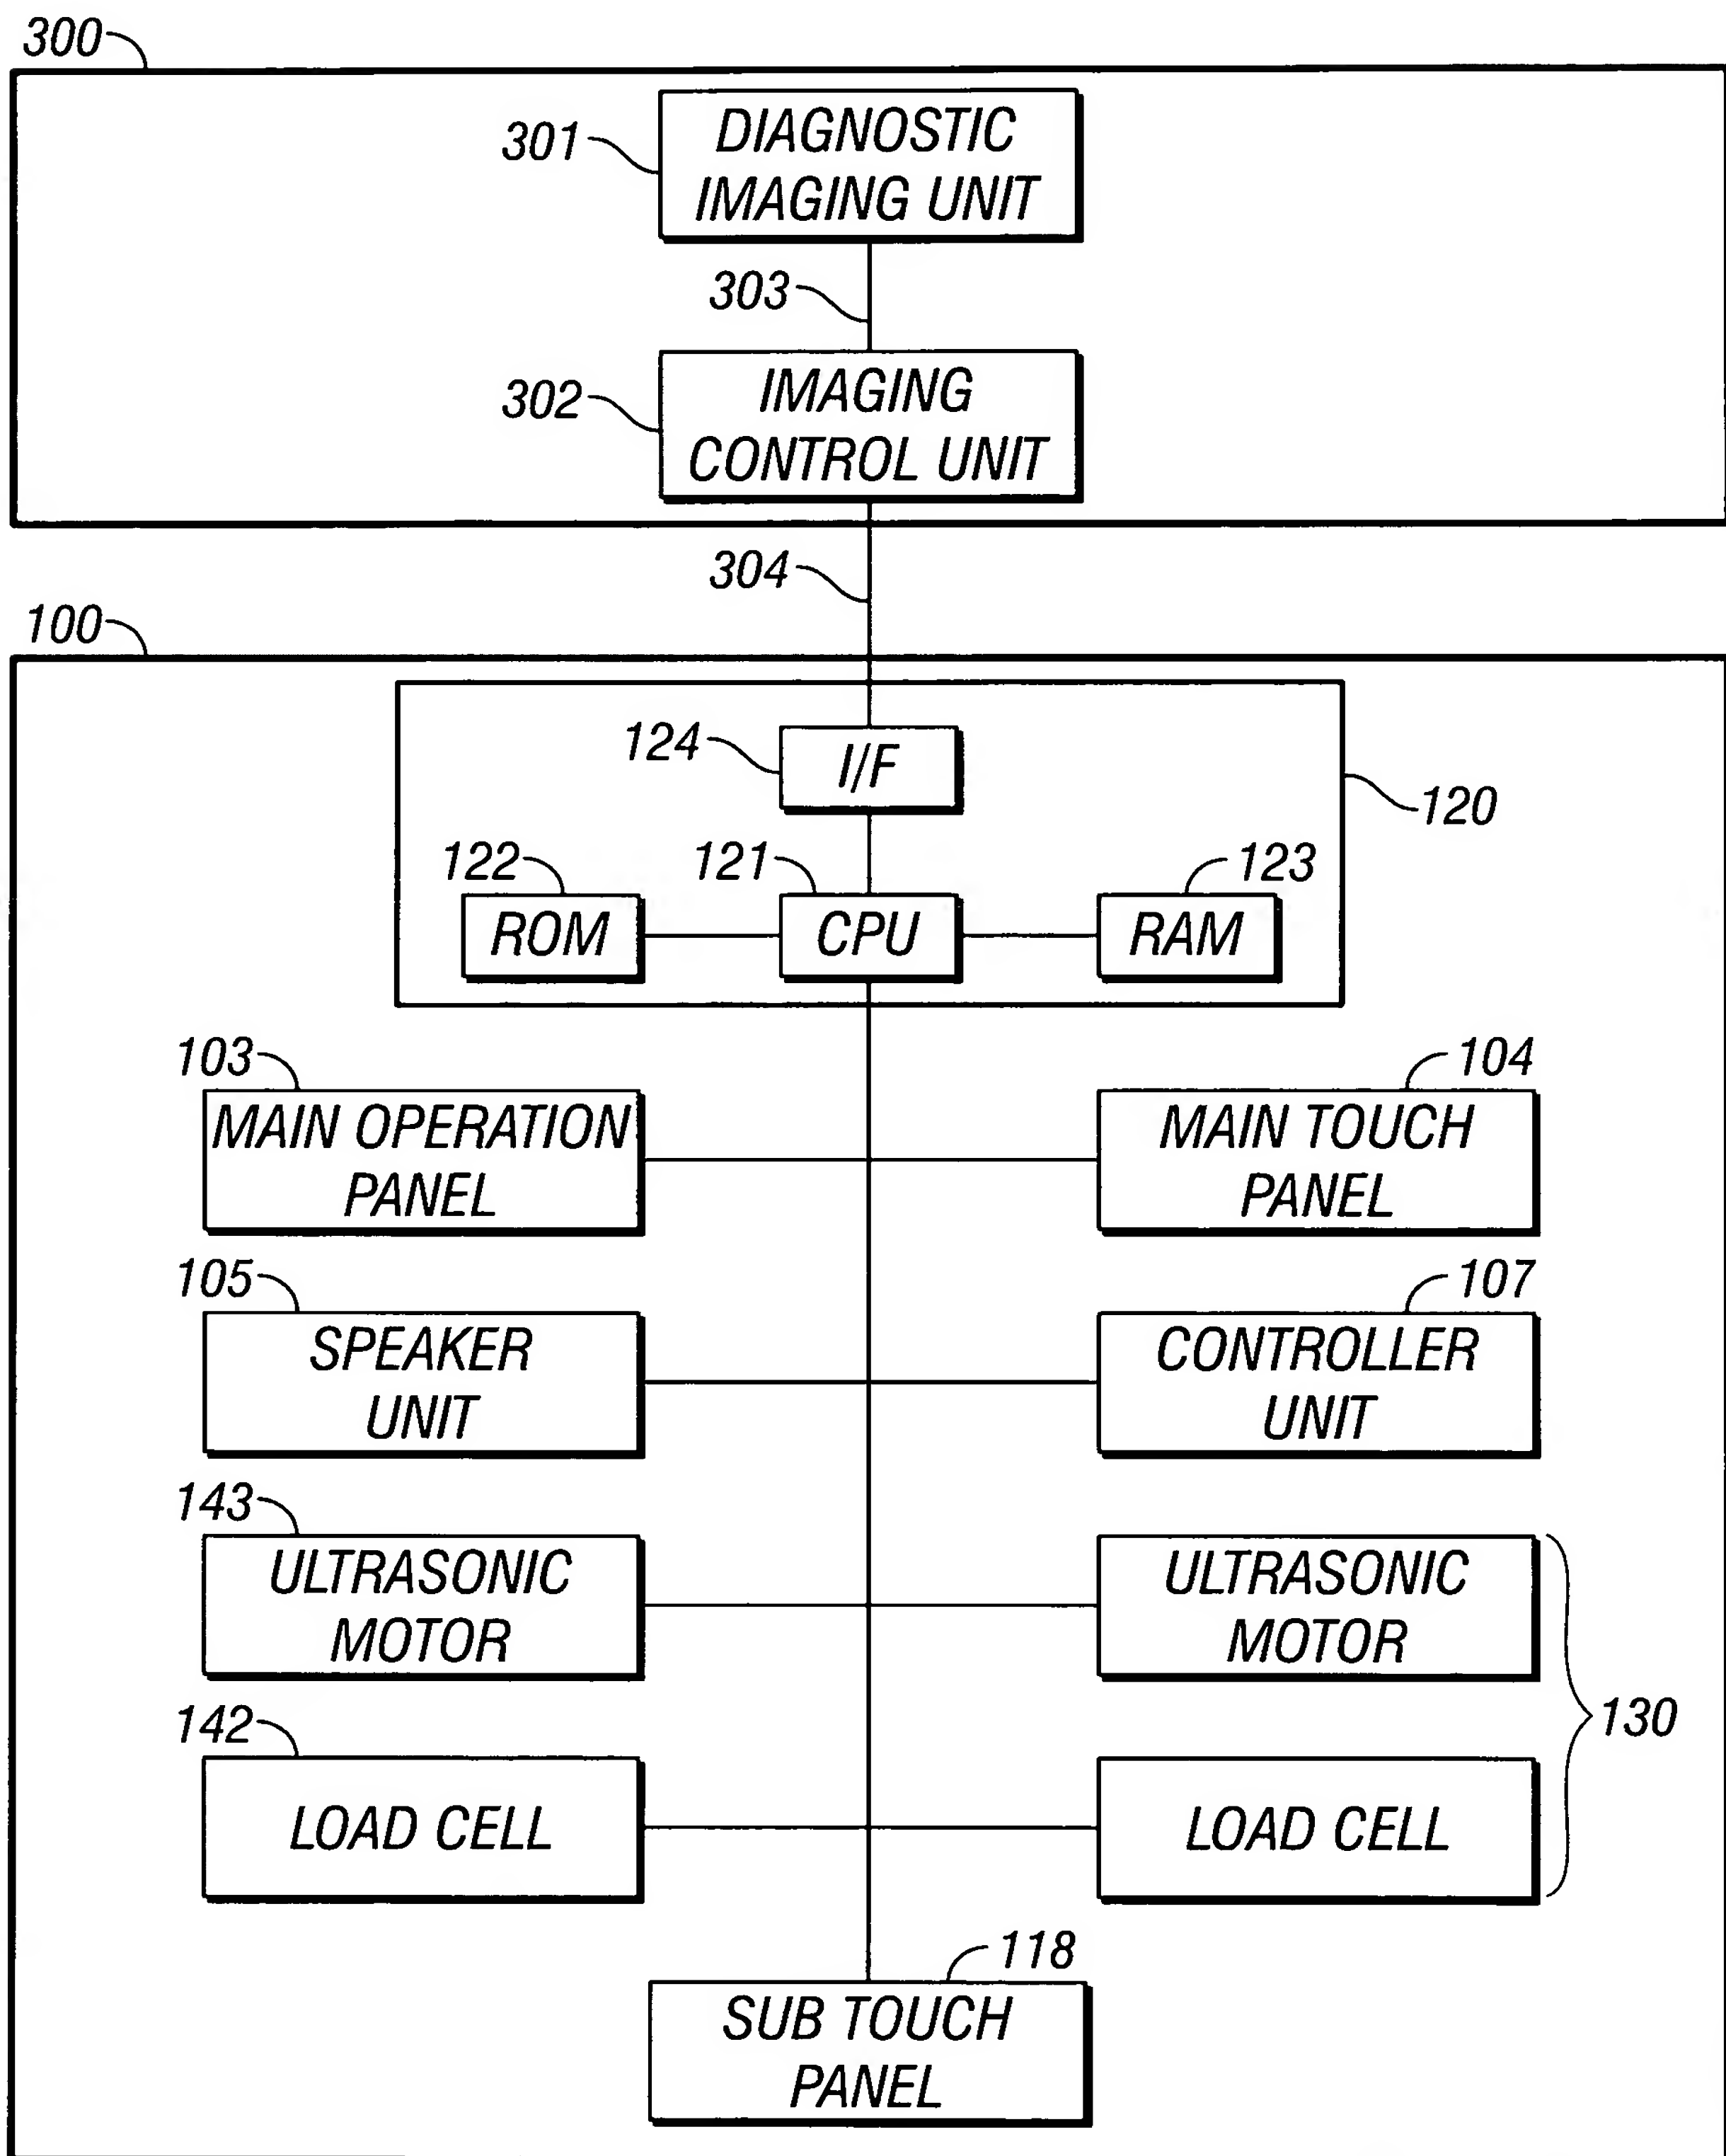


FIG. 5

6/16

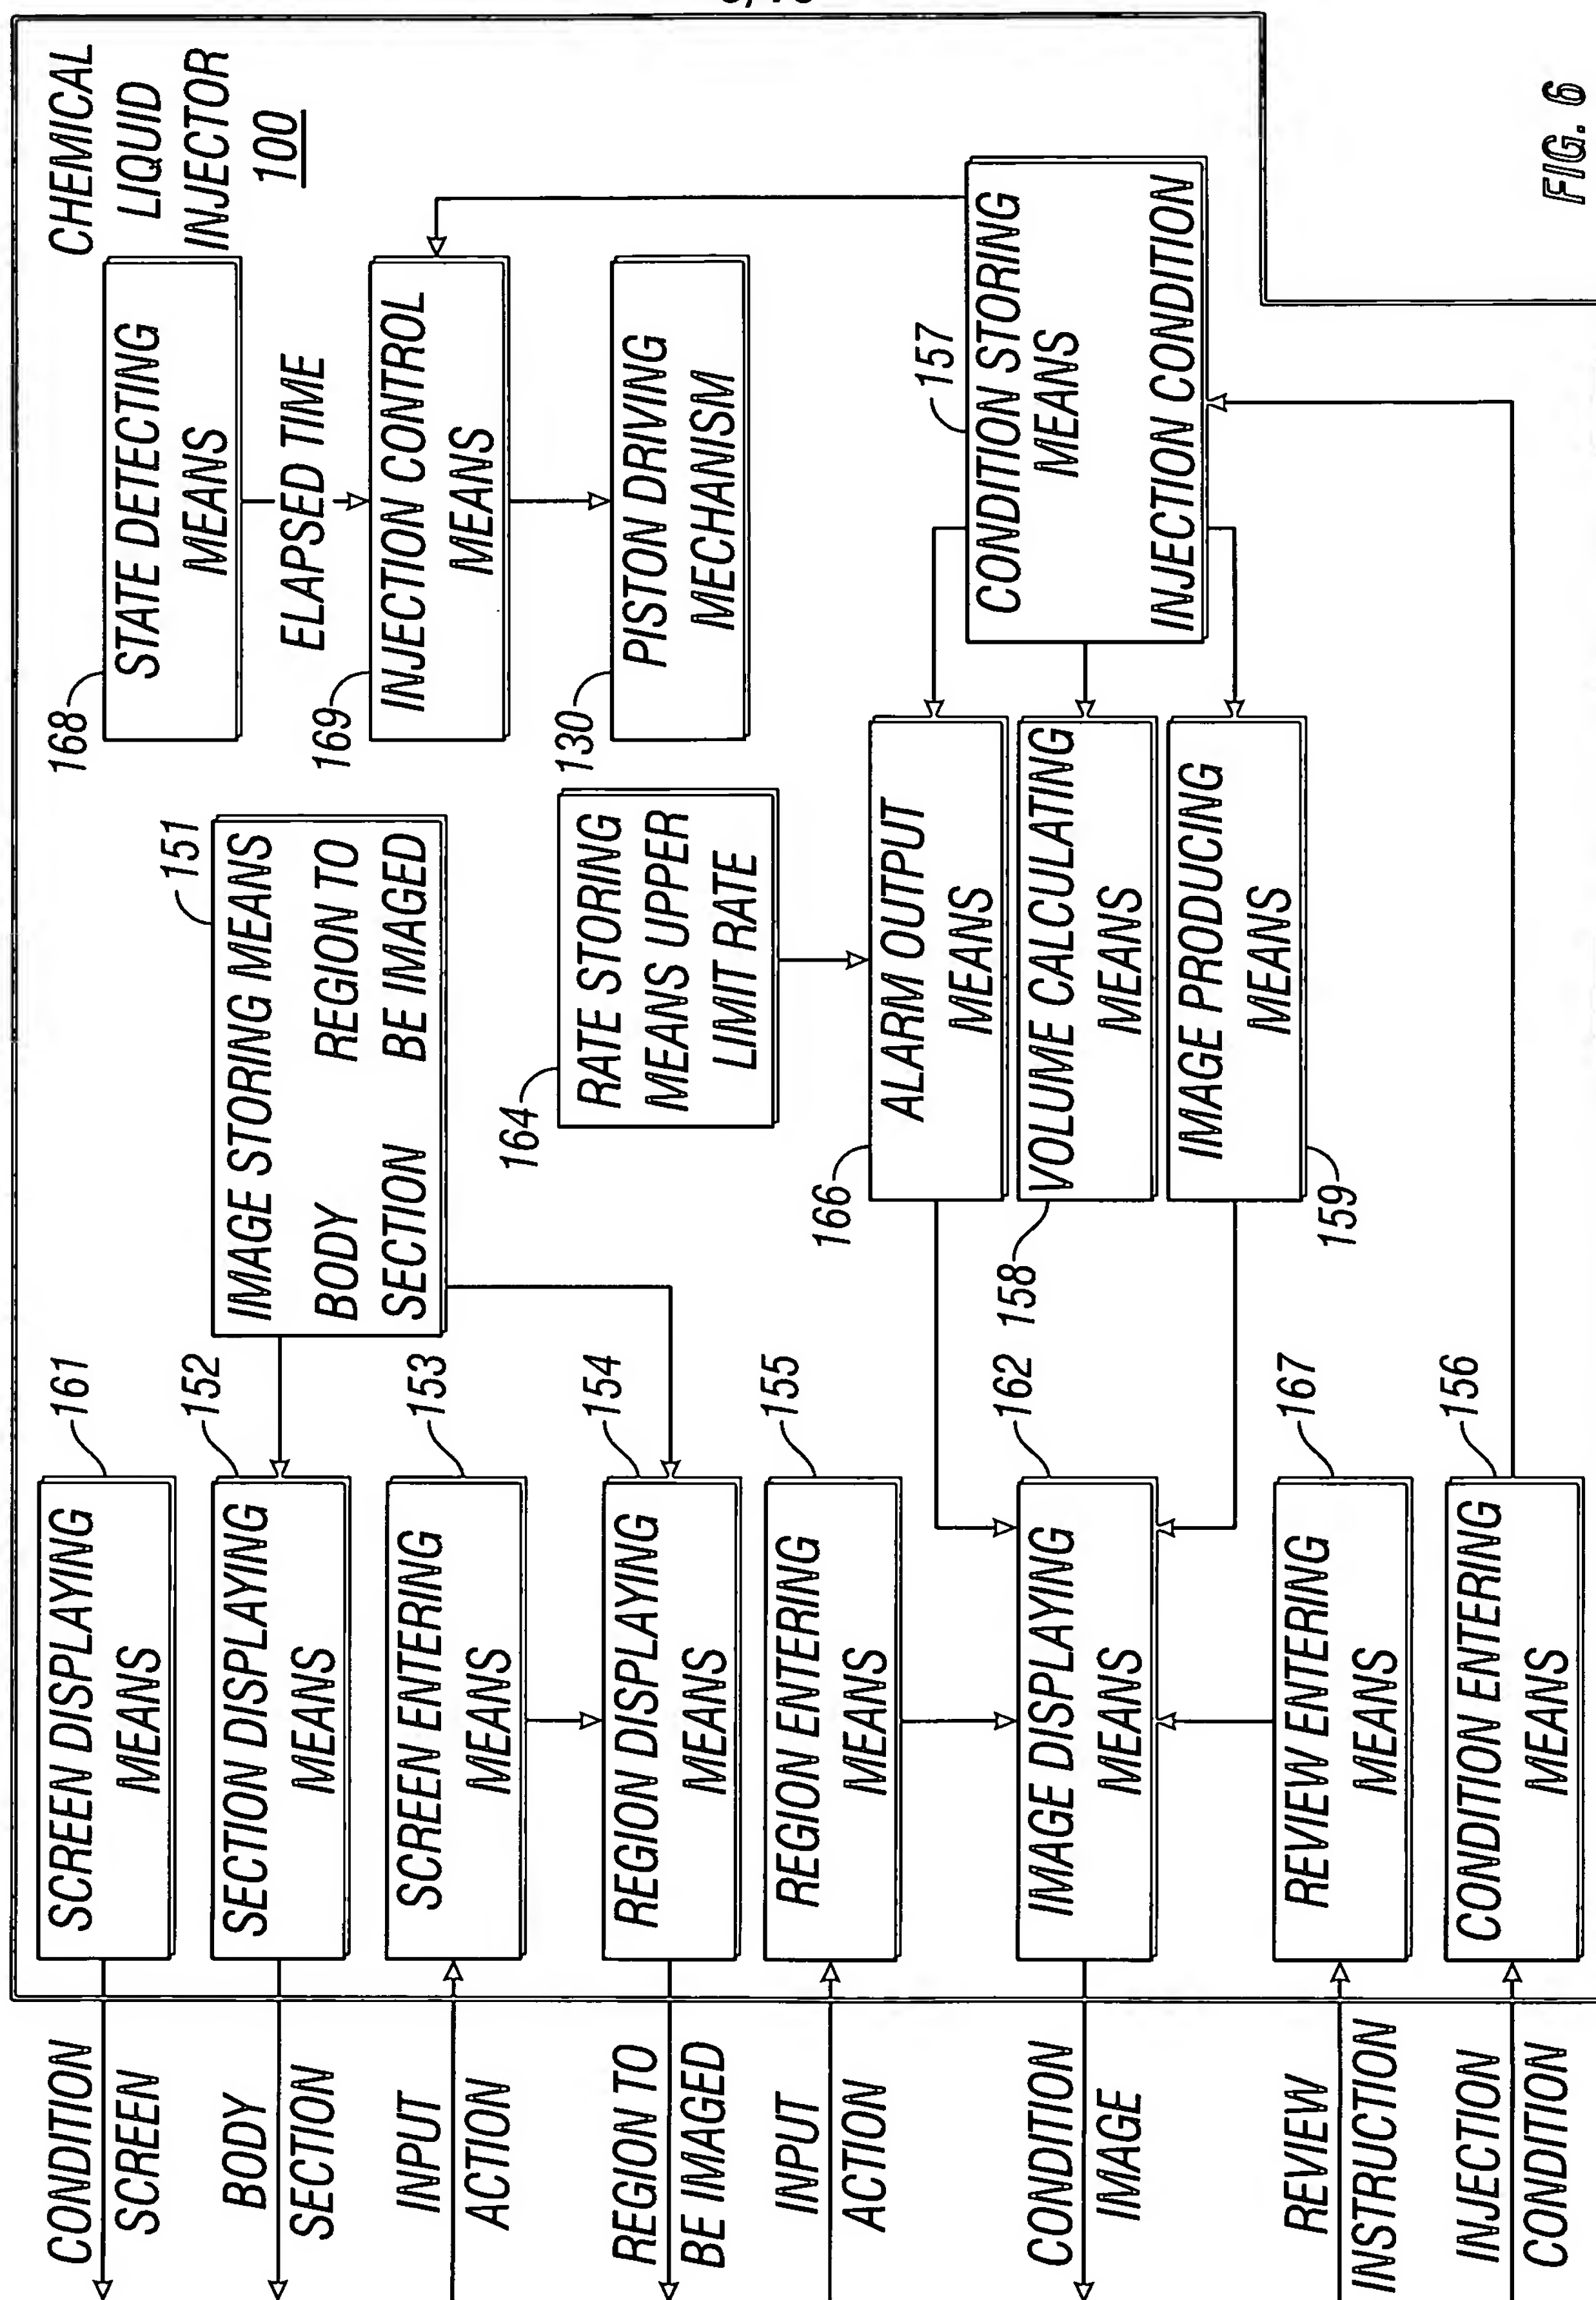


FIG. 6

7/16

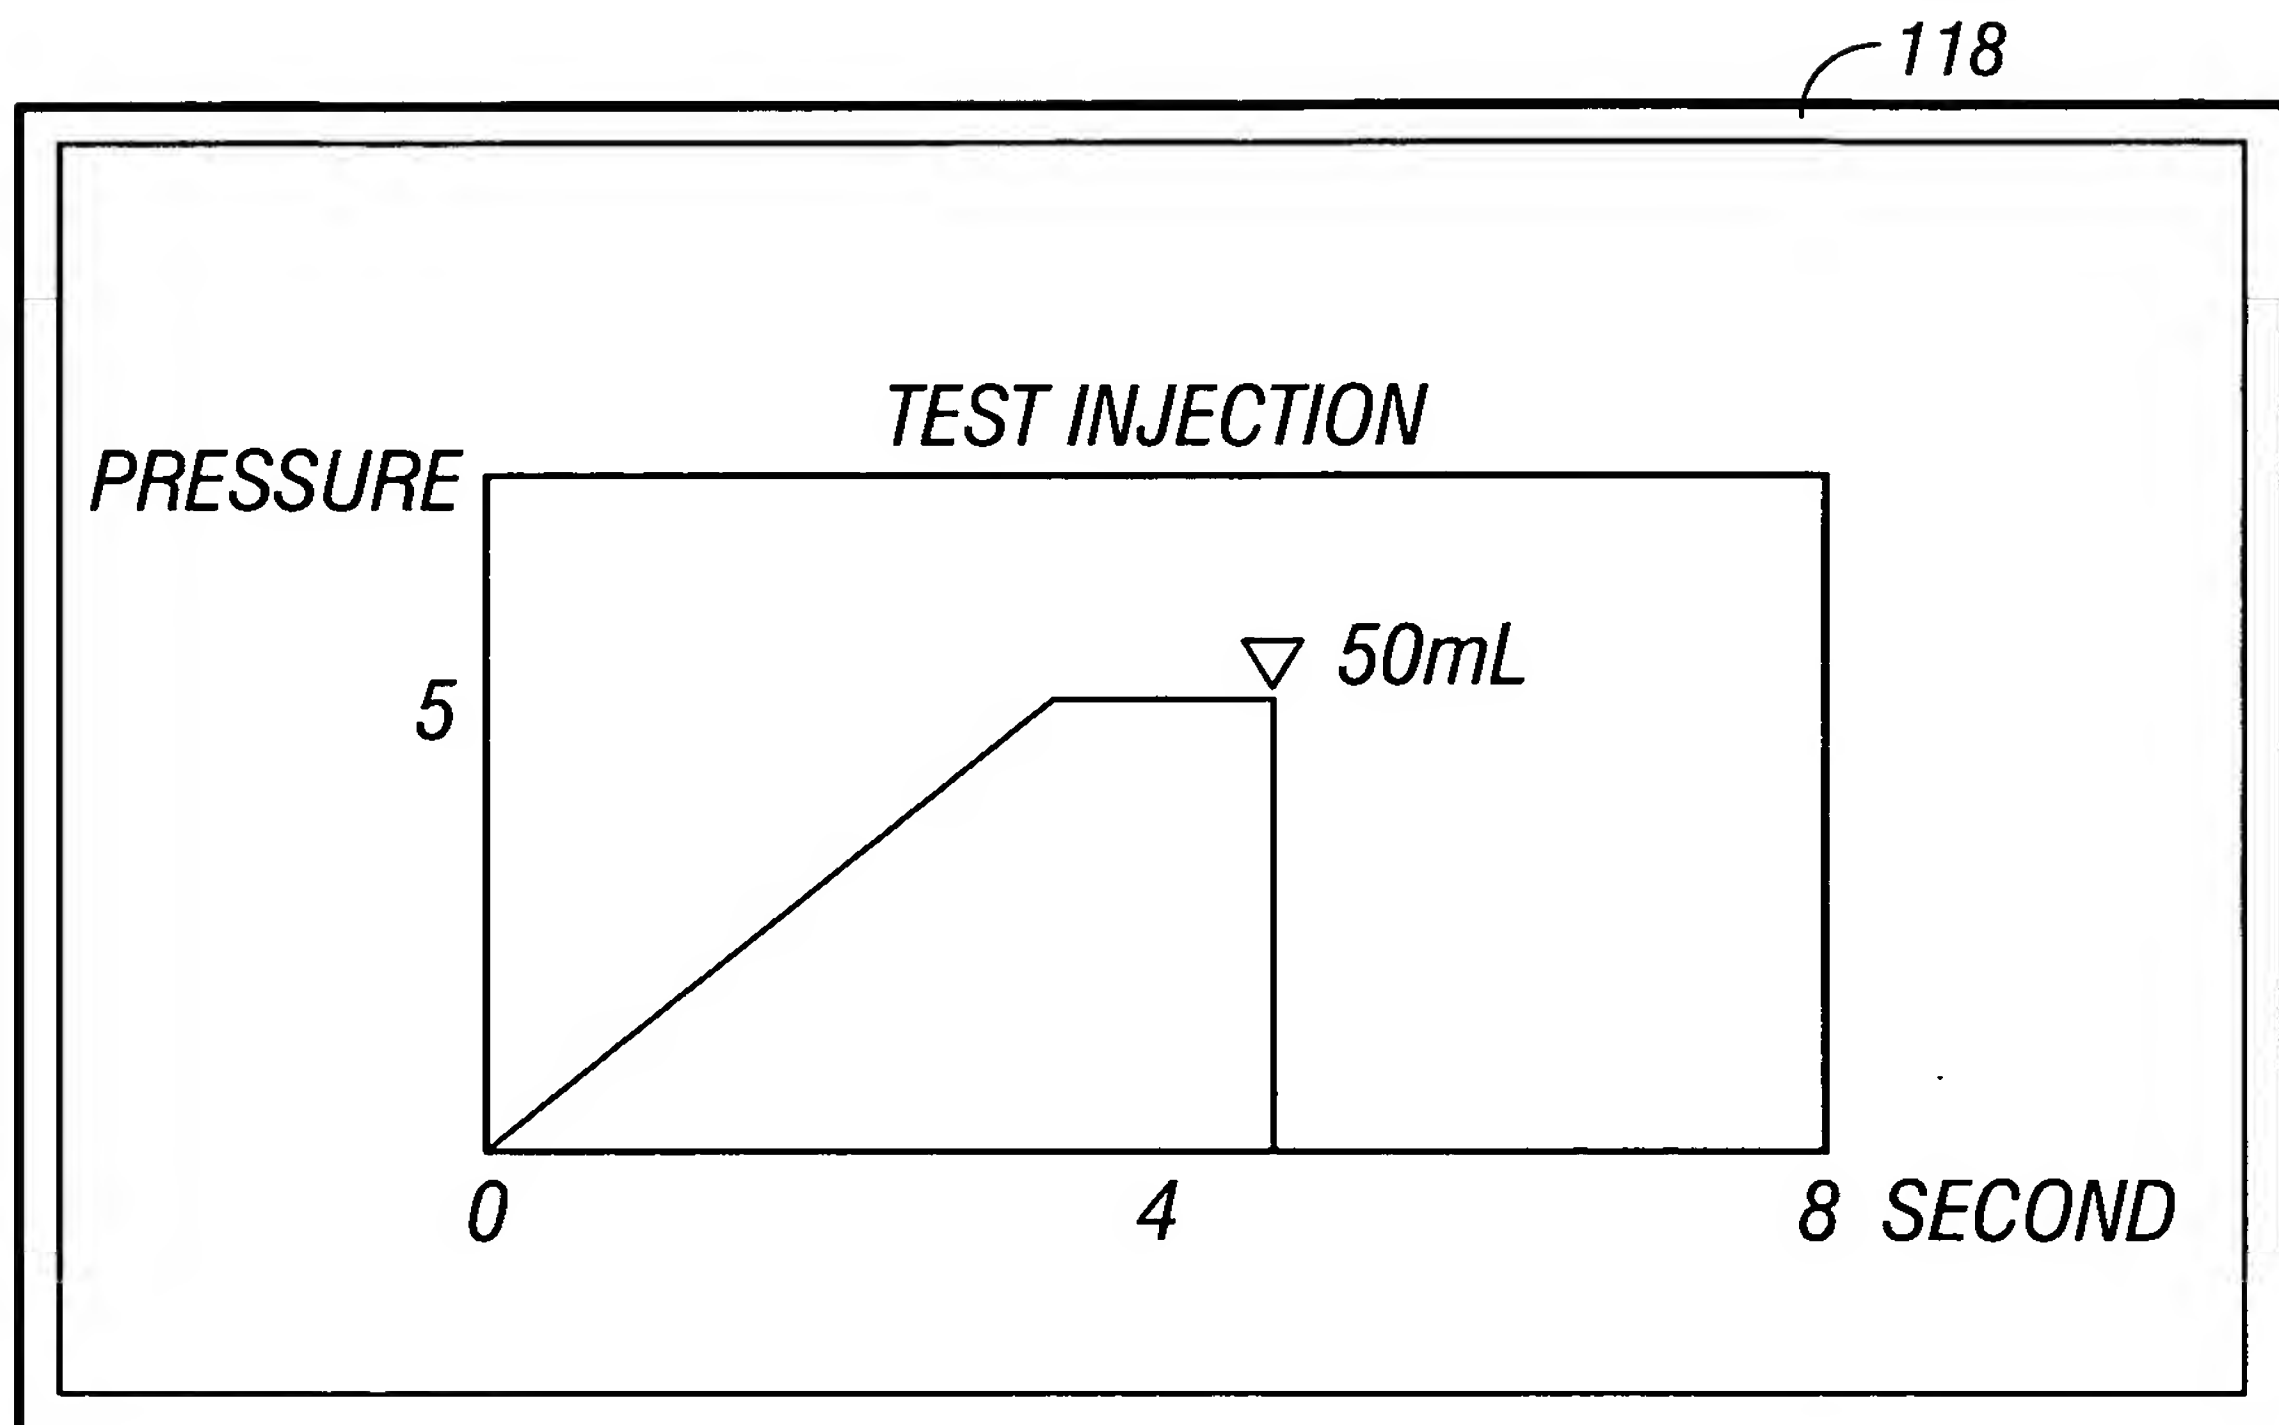


FIG. 7

8/16

104

BODY SECTIONS

ENTER

**REGION(S)
TO BE IMAGED**

RATE

0 **TIME**

FIG. 8

104

BODY SECTIONS

ENTER

**REGION(S)
TO BE IMAGED**

CHEST PART

LUNG PART

HEART PART

RATE


0 **TIME**

FIG. 9

9/16

104


BODY SECTIONS

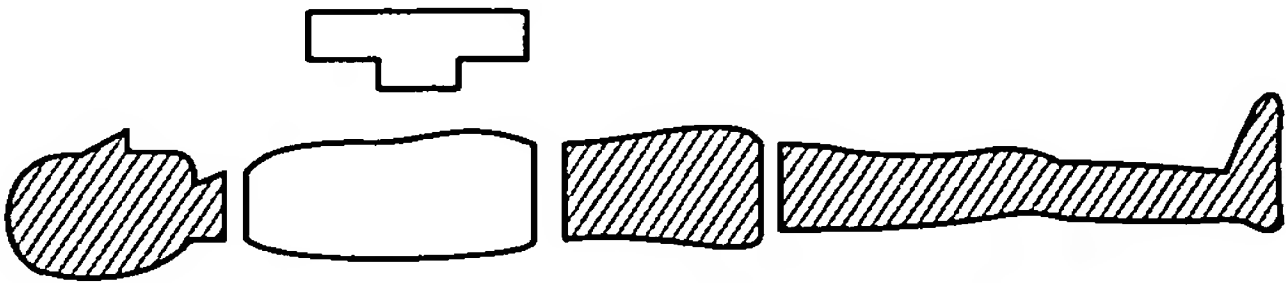


ENTER

REGION(S)
TO BE IMAGED

CHEST PART


 LUNG PART


 HEART PART


RATE

	RATE	VOLUME	
<div style="border: 1px solid black; border-radius: 10px; padding: 5px; margin-bottom: 10px; width: 80%; margin-left: auto; margin-right: auto;"> RATE 2.0 mL/sec VOLUME 40 ml </div>	0	0:20	0:50
<div style="border: 1px solid black; border-radius: 10px; padding: 5px; margin-bottom: 10px; width: 80%; margin-left: auto; margin-right: auto;"> RATE 4.0 mL/sec VOLUME 120 ml </div>			TIME

FIG. 10

104


BODY SECTIONS

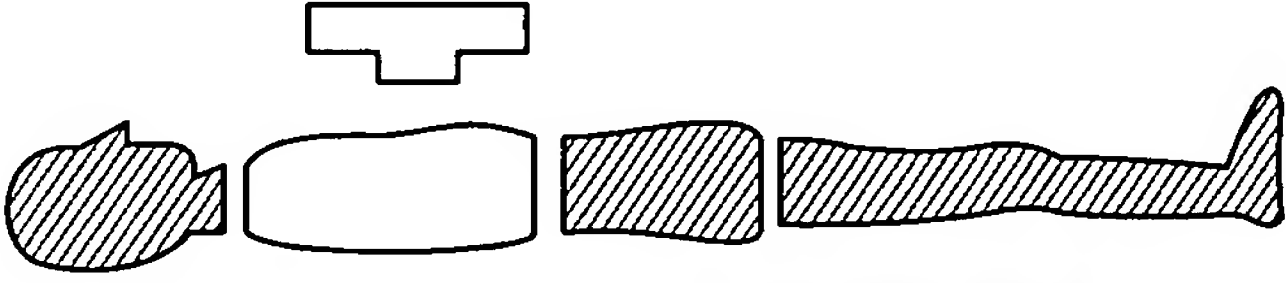


ENTER

REGION(S)
TO BE IMAGED

CHEST PART



 LUNG PART


 HEART PART

RATE

	RATE mL/sec	VOLUME ml	
<div style="border: 1px solid black; border-radius: 10px; padding: 5px; margin-bottom: 10px; width: 80%; margin-left: auto; margin-right: auto;"> RATE 2.0 VOLUME 40 </div>	0	0:20	0:50
<div style="border: 1px solid black; border-radius: 10px; padding: 5px; margin-bottom: 10px; width: 80%; margin-left: auto; margin-right: auto;"> RATE 4.0 VOLUME 120 </div>			TIME

FIG. 11

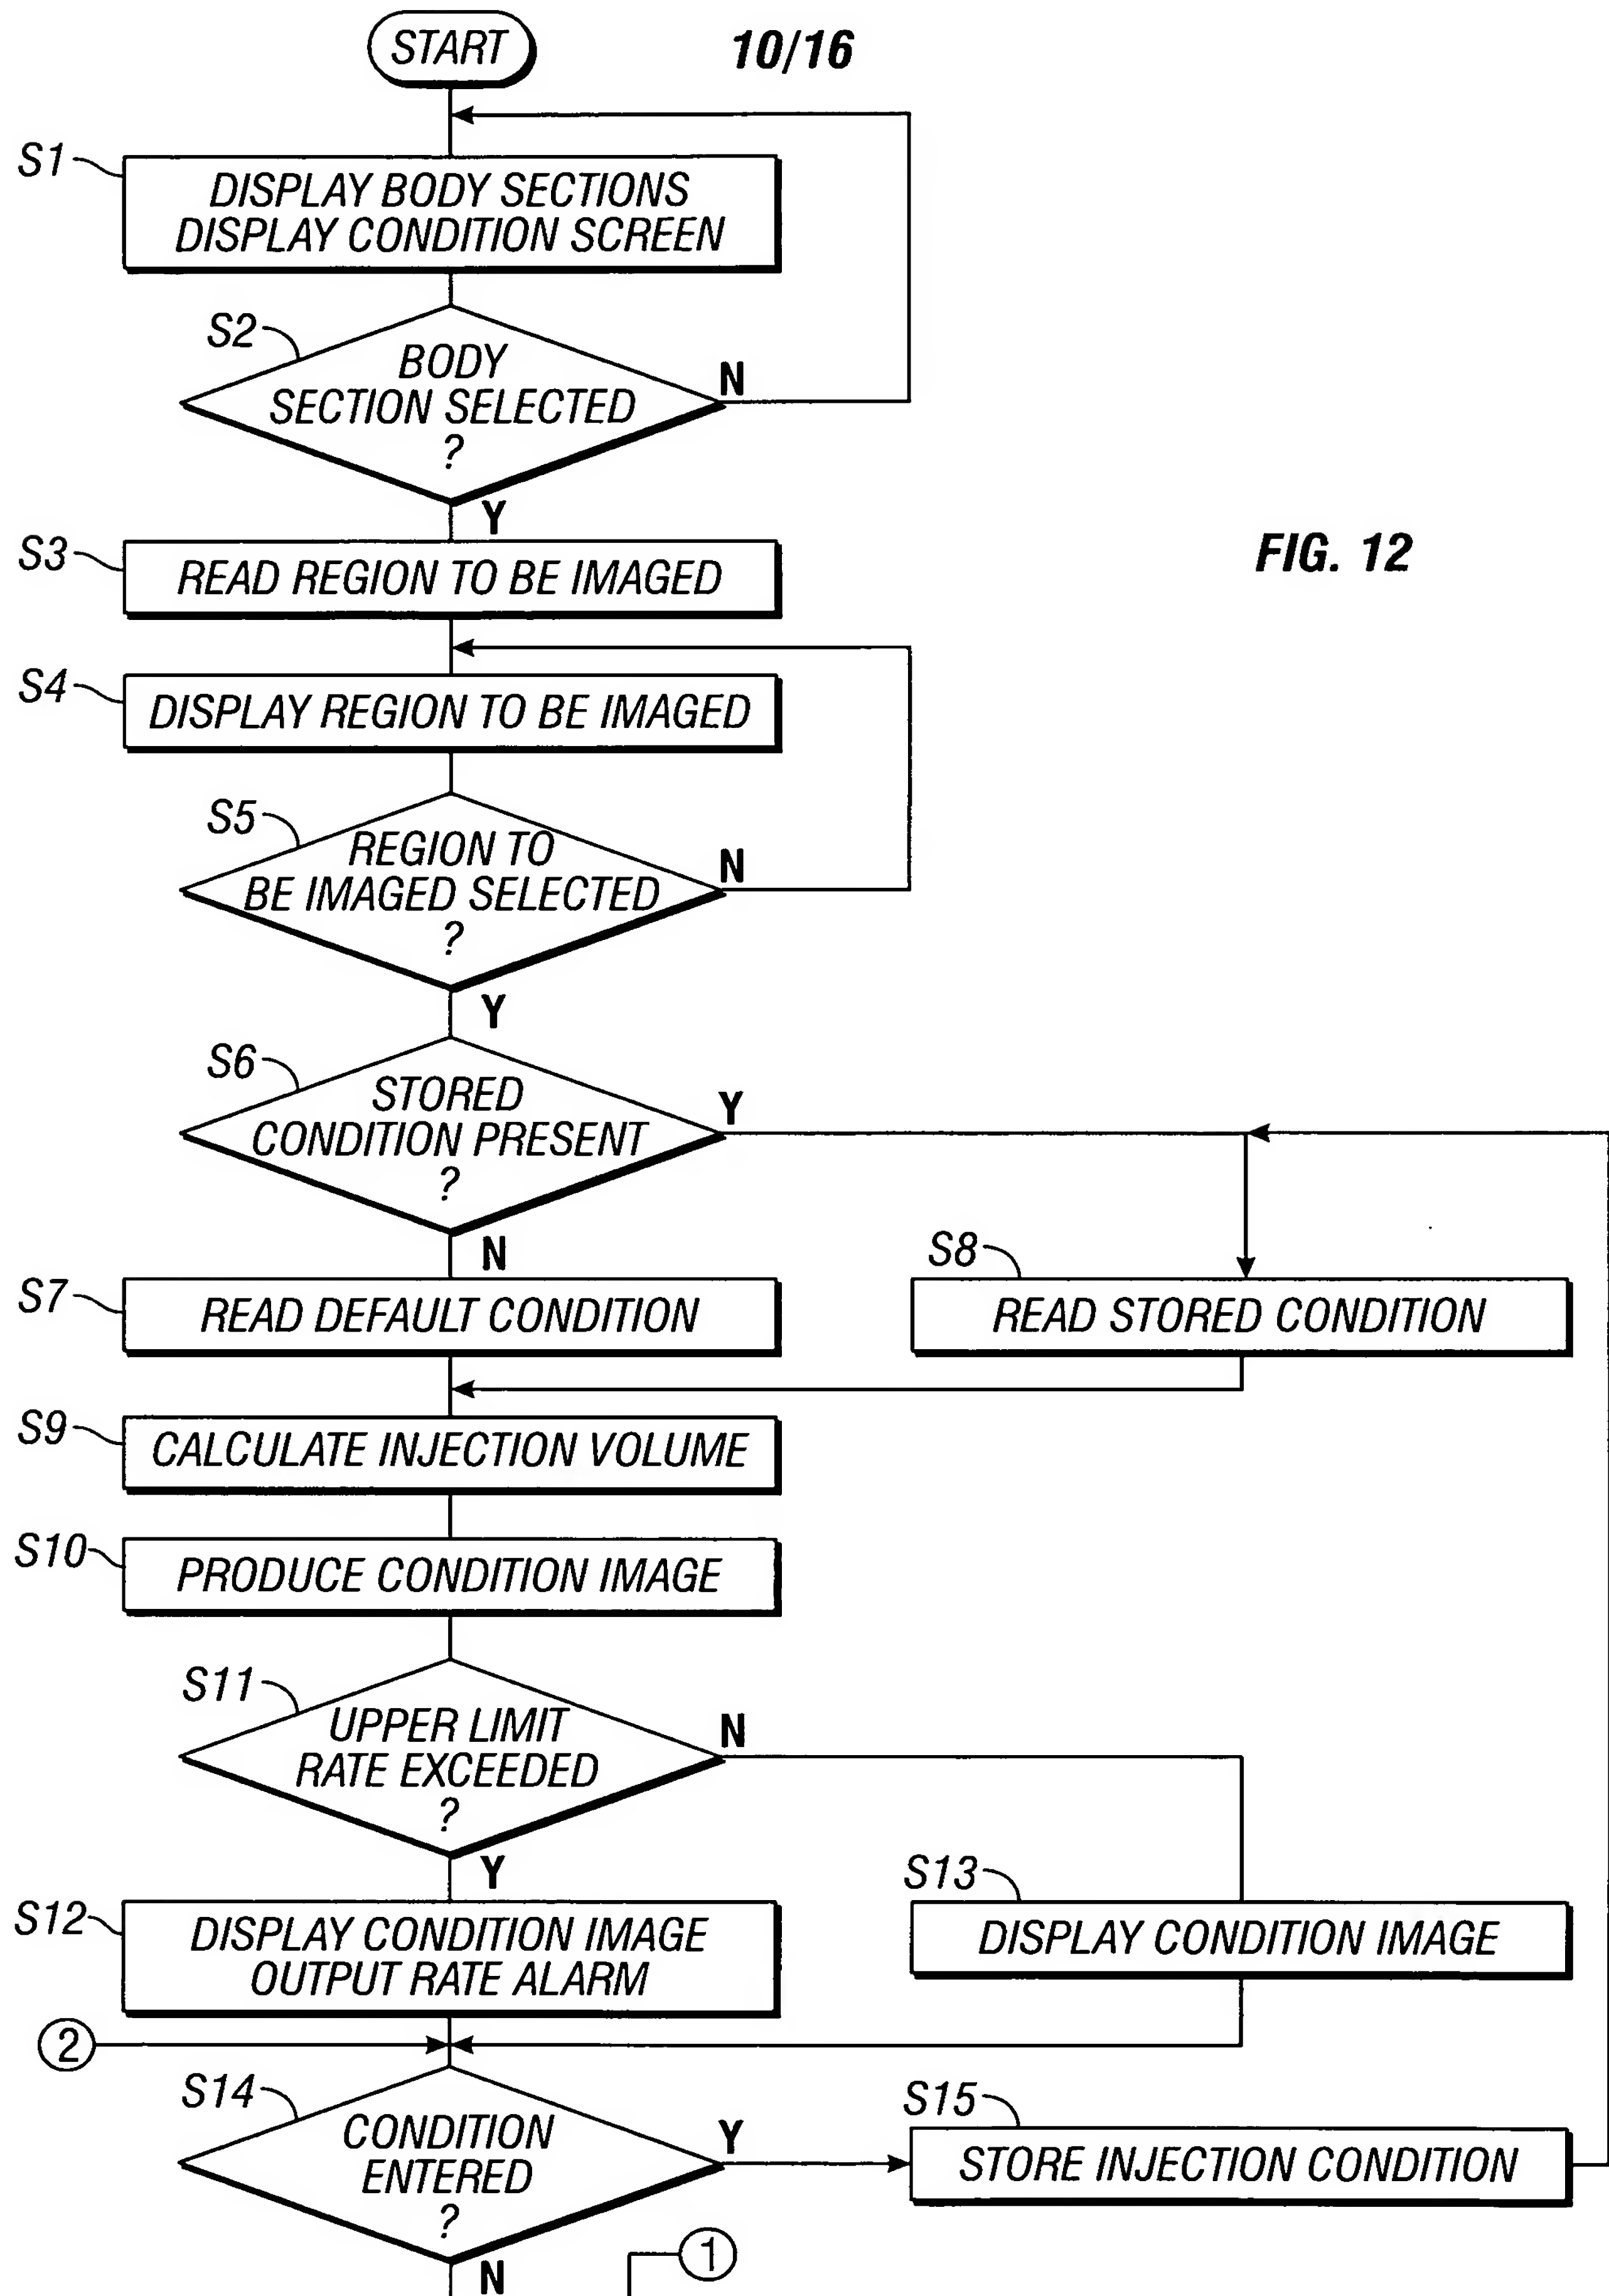

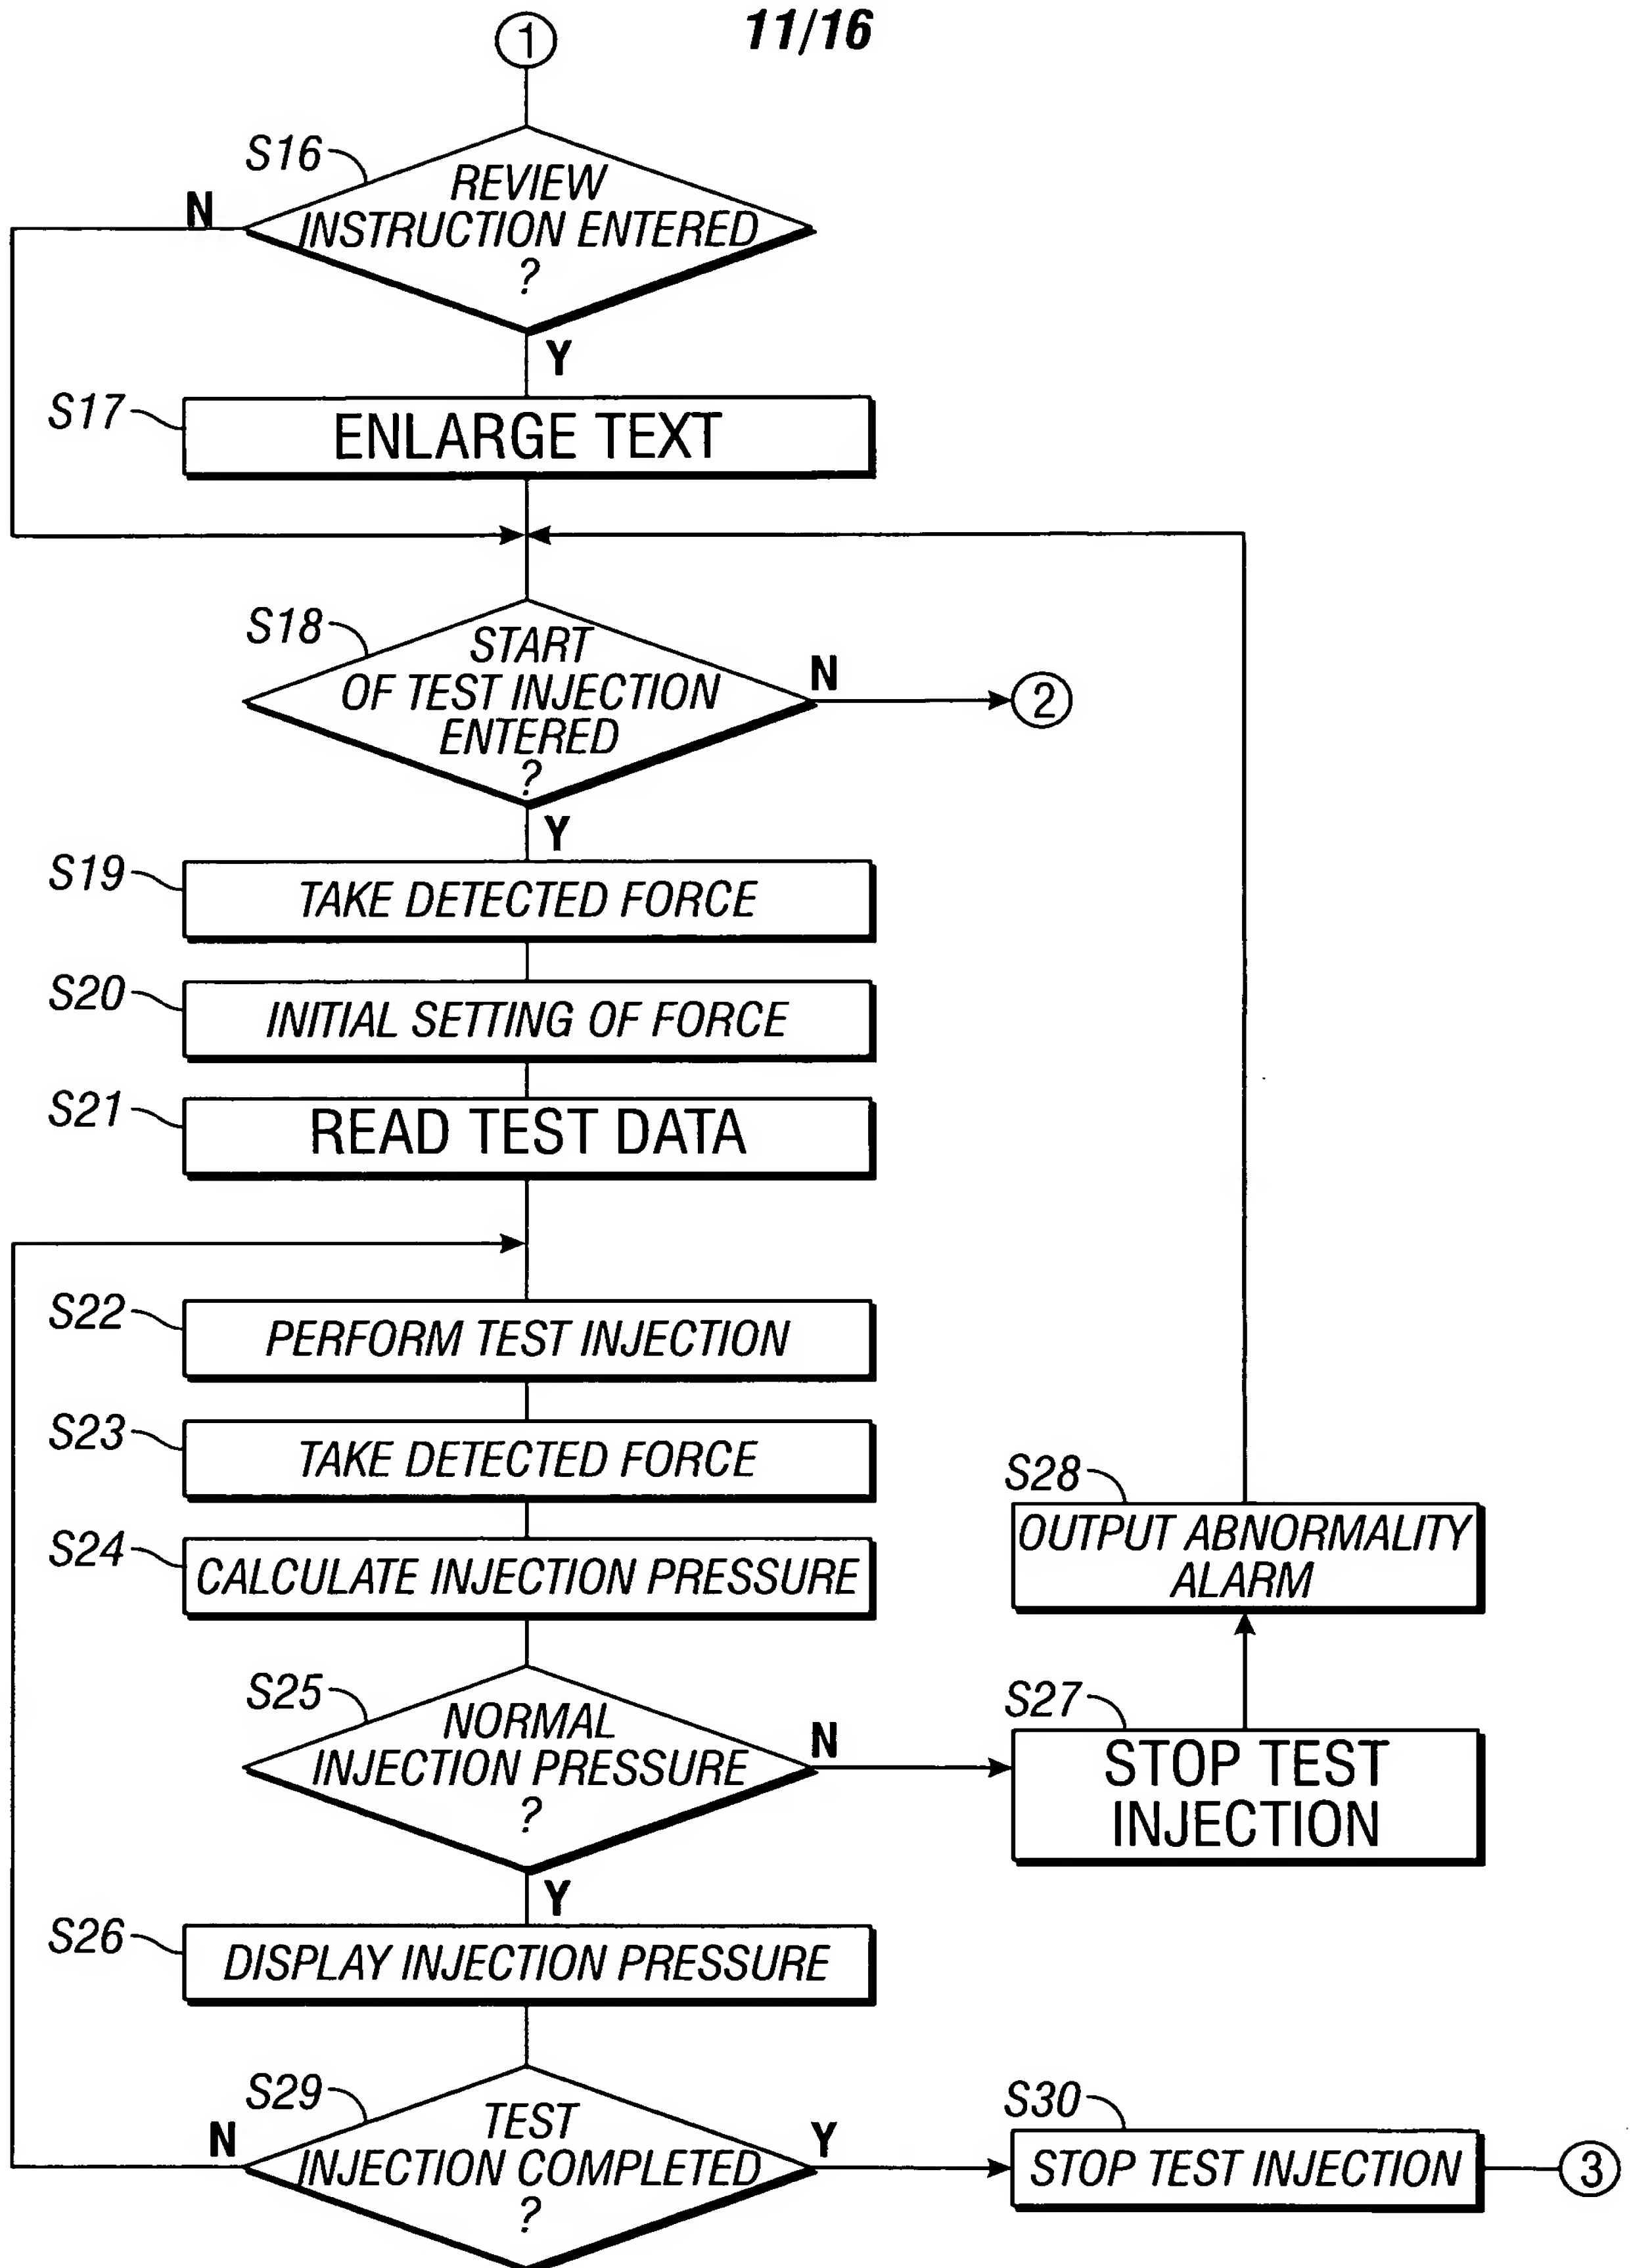


FIG. 13

12/16

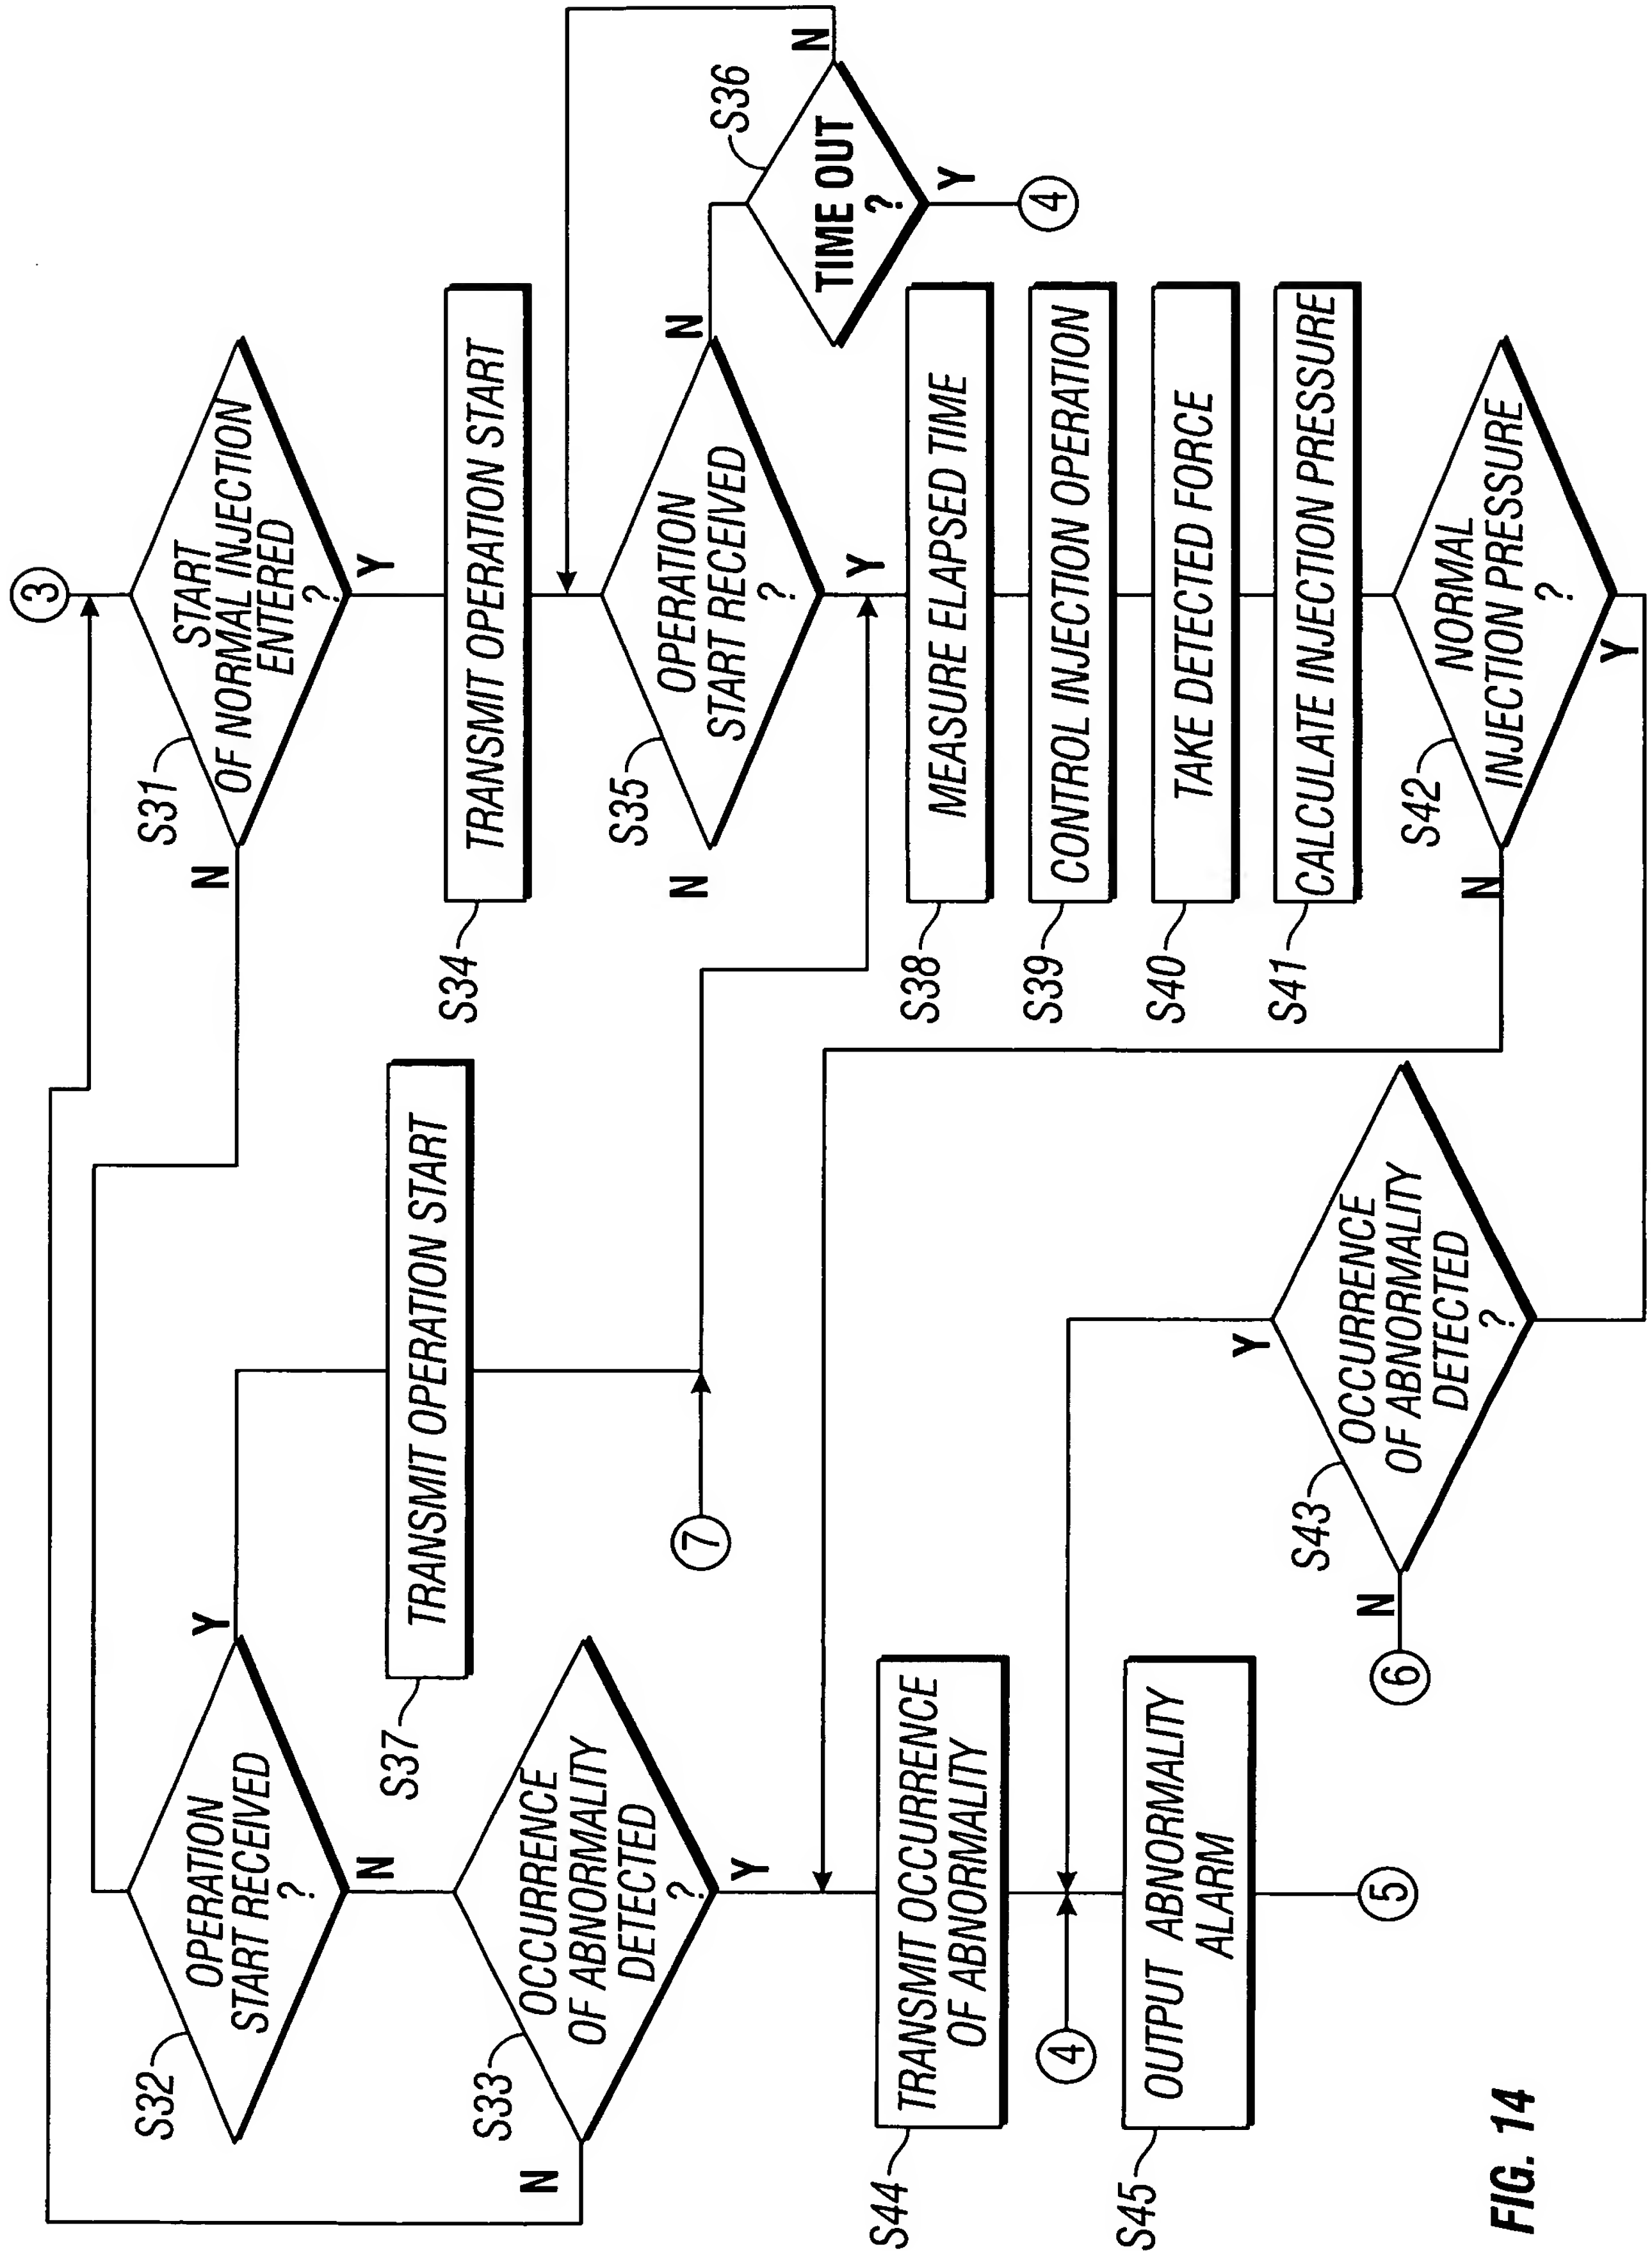


FIG. 14

13/16

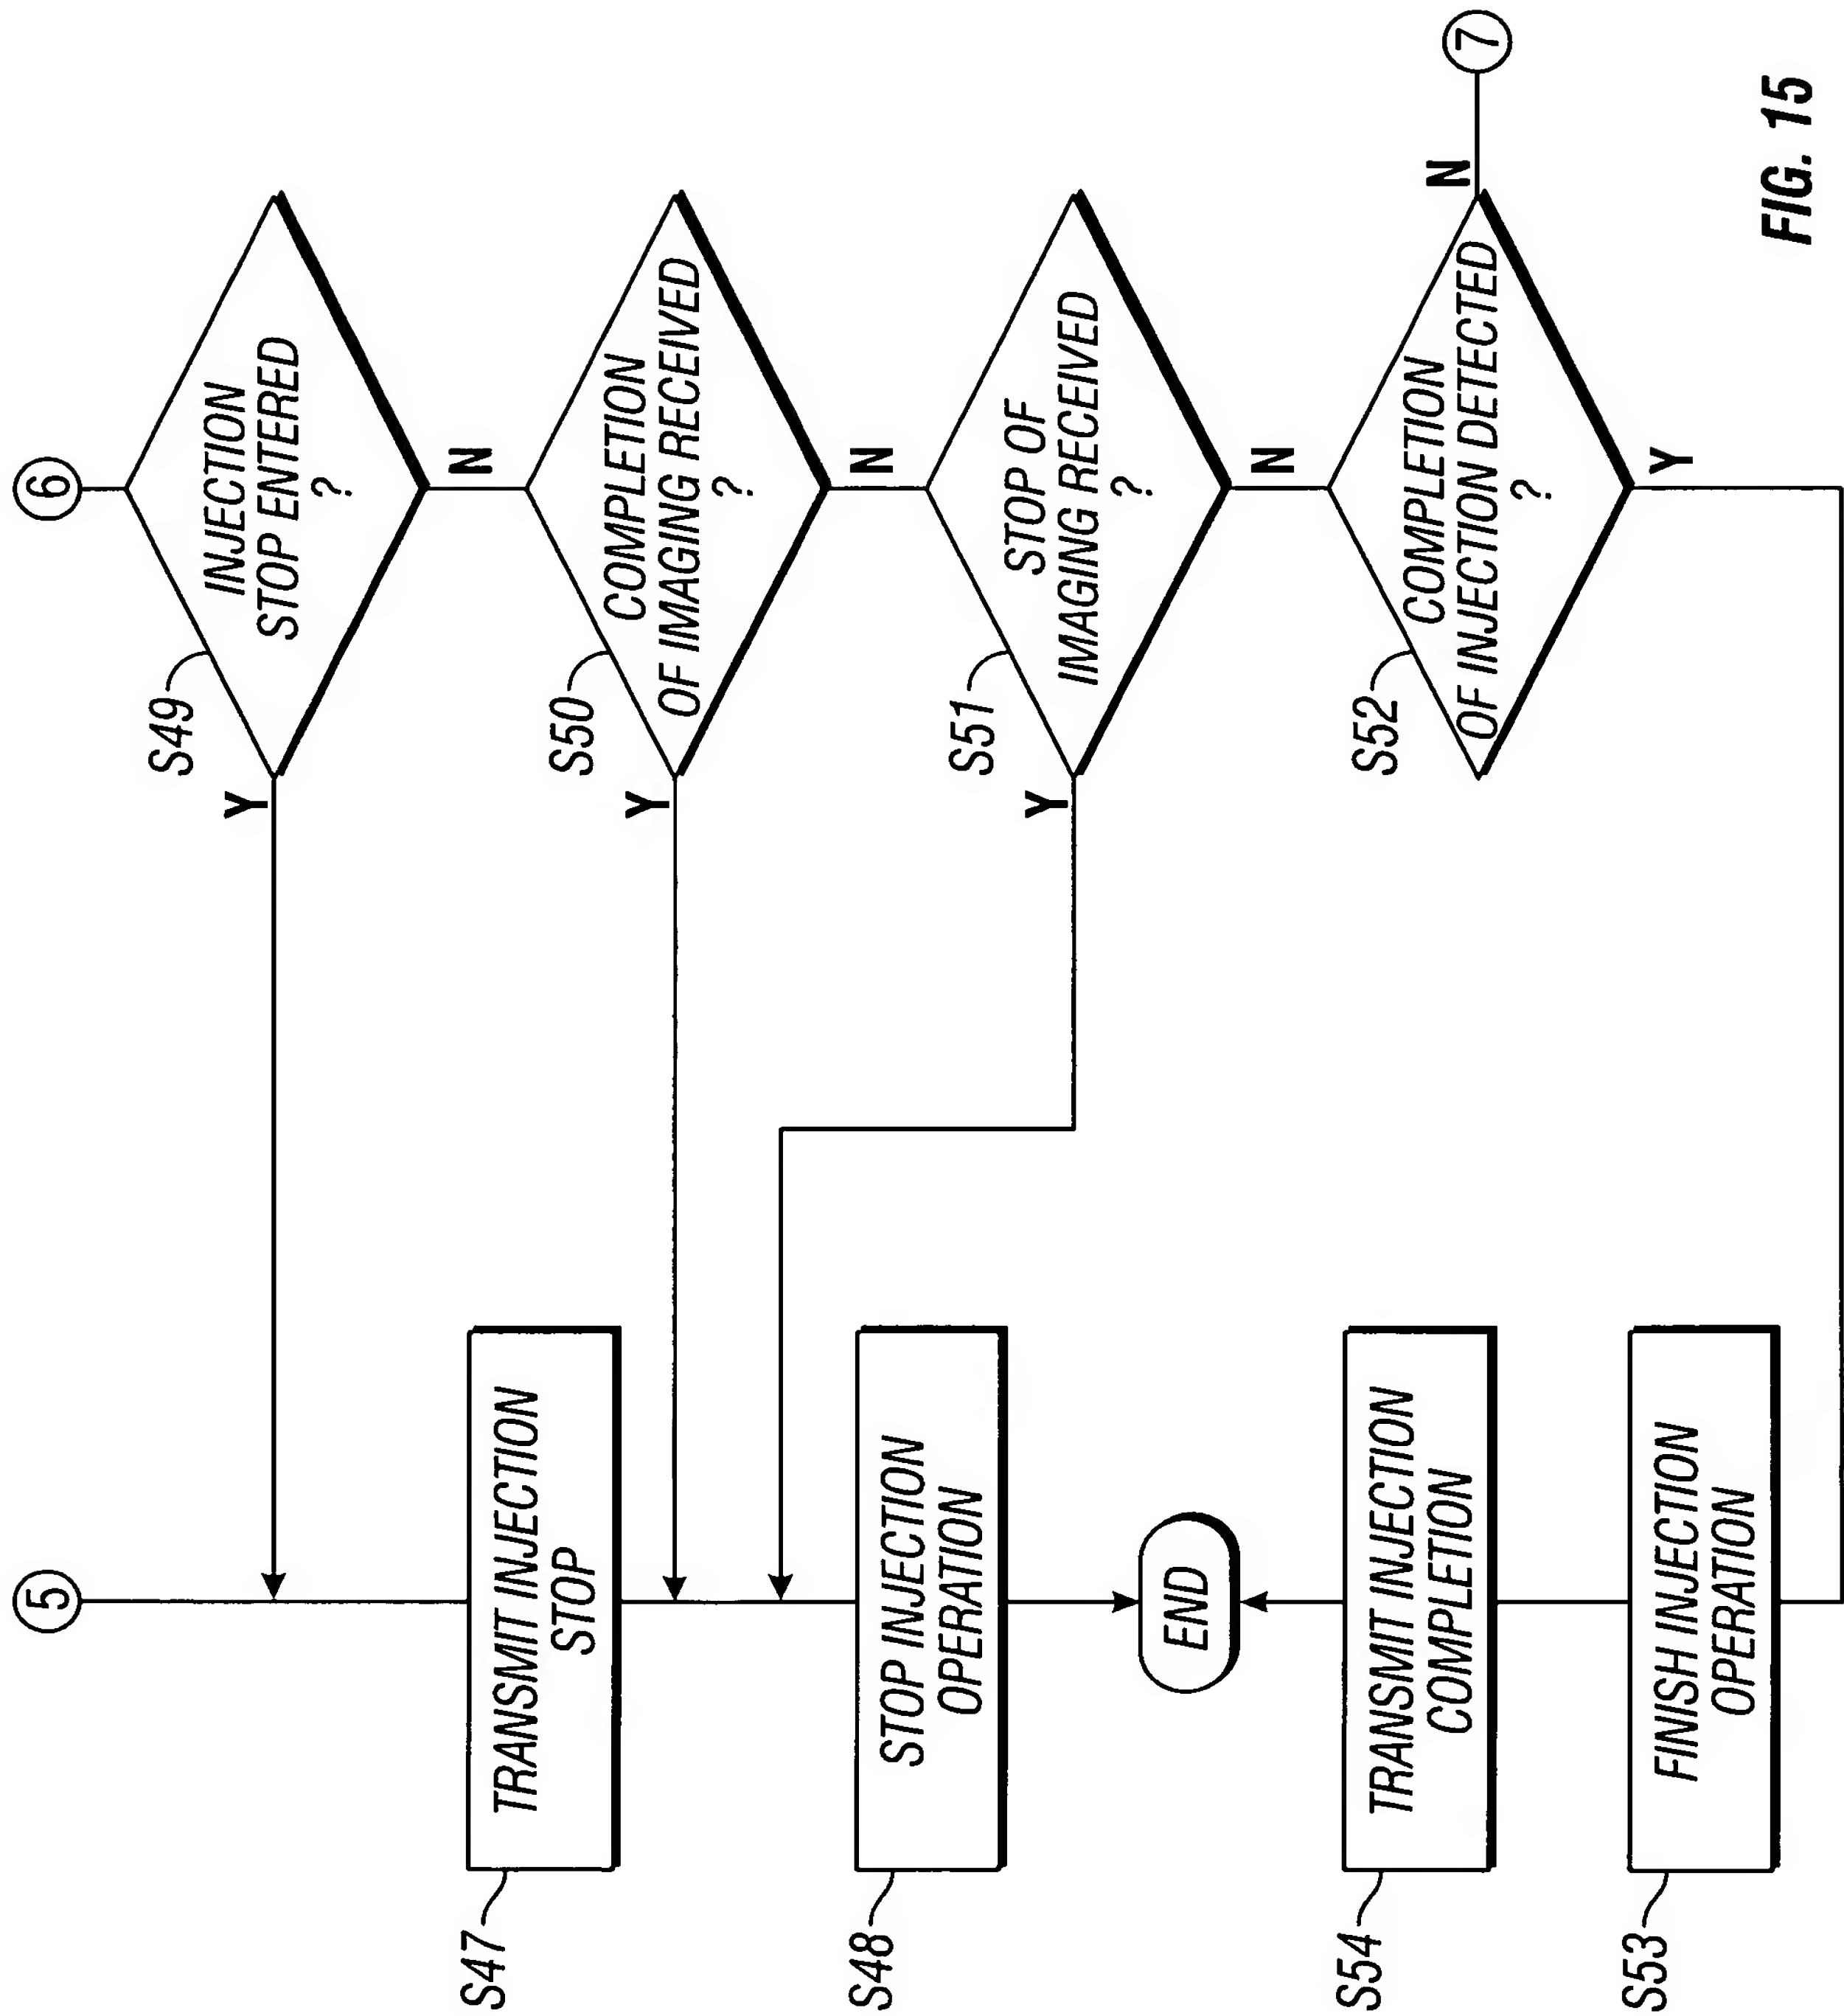


FIG. 15

14/16

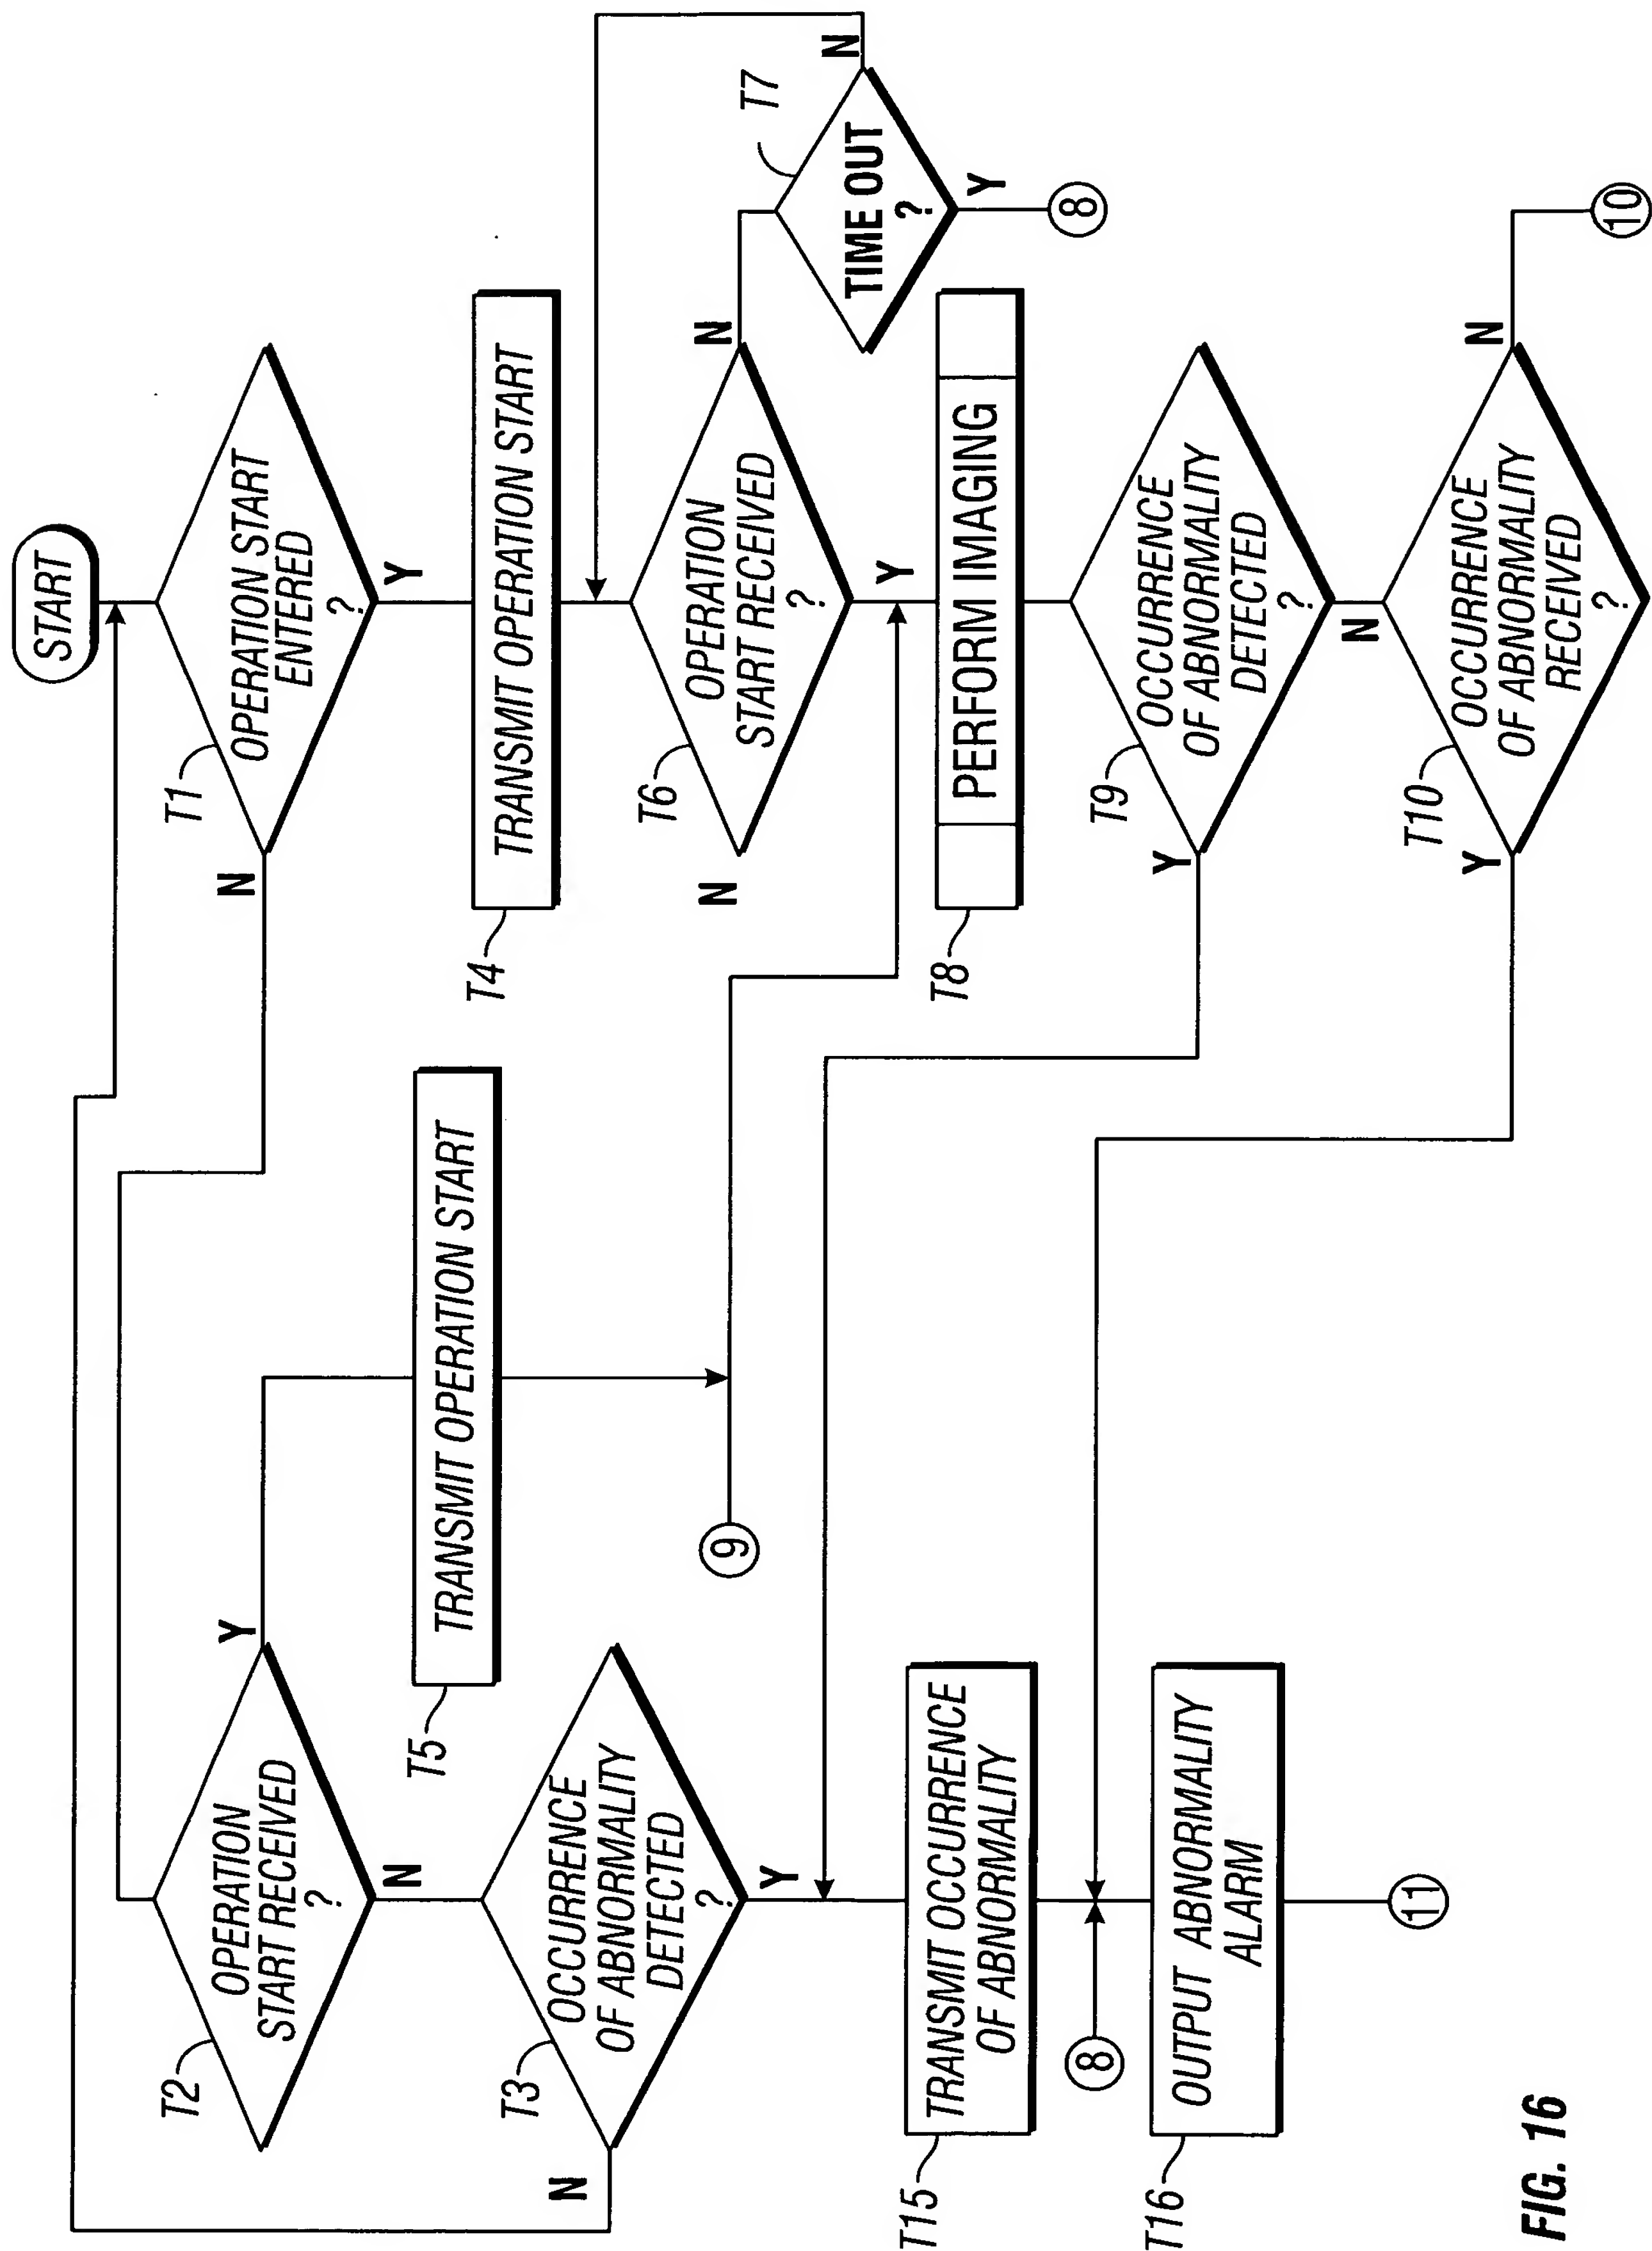


FIG. 16

15/16

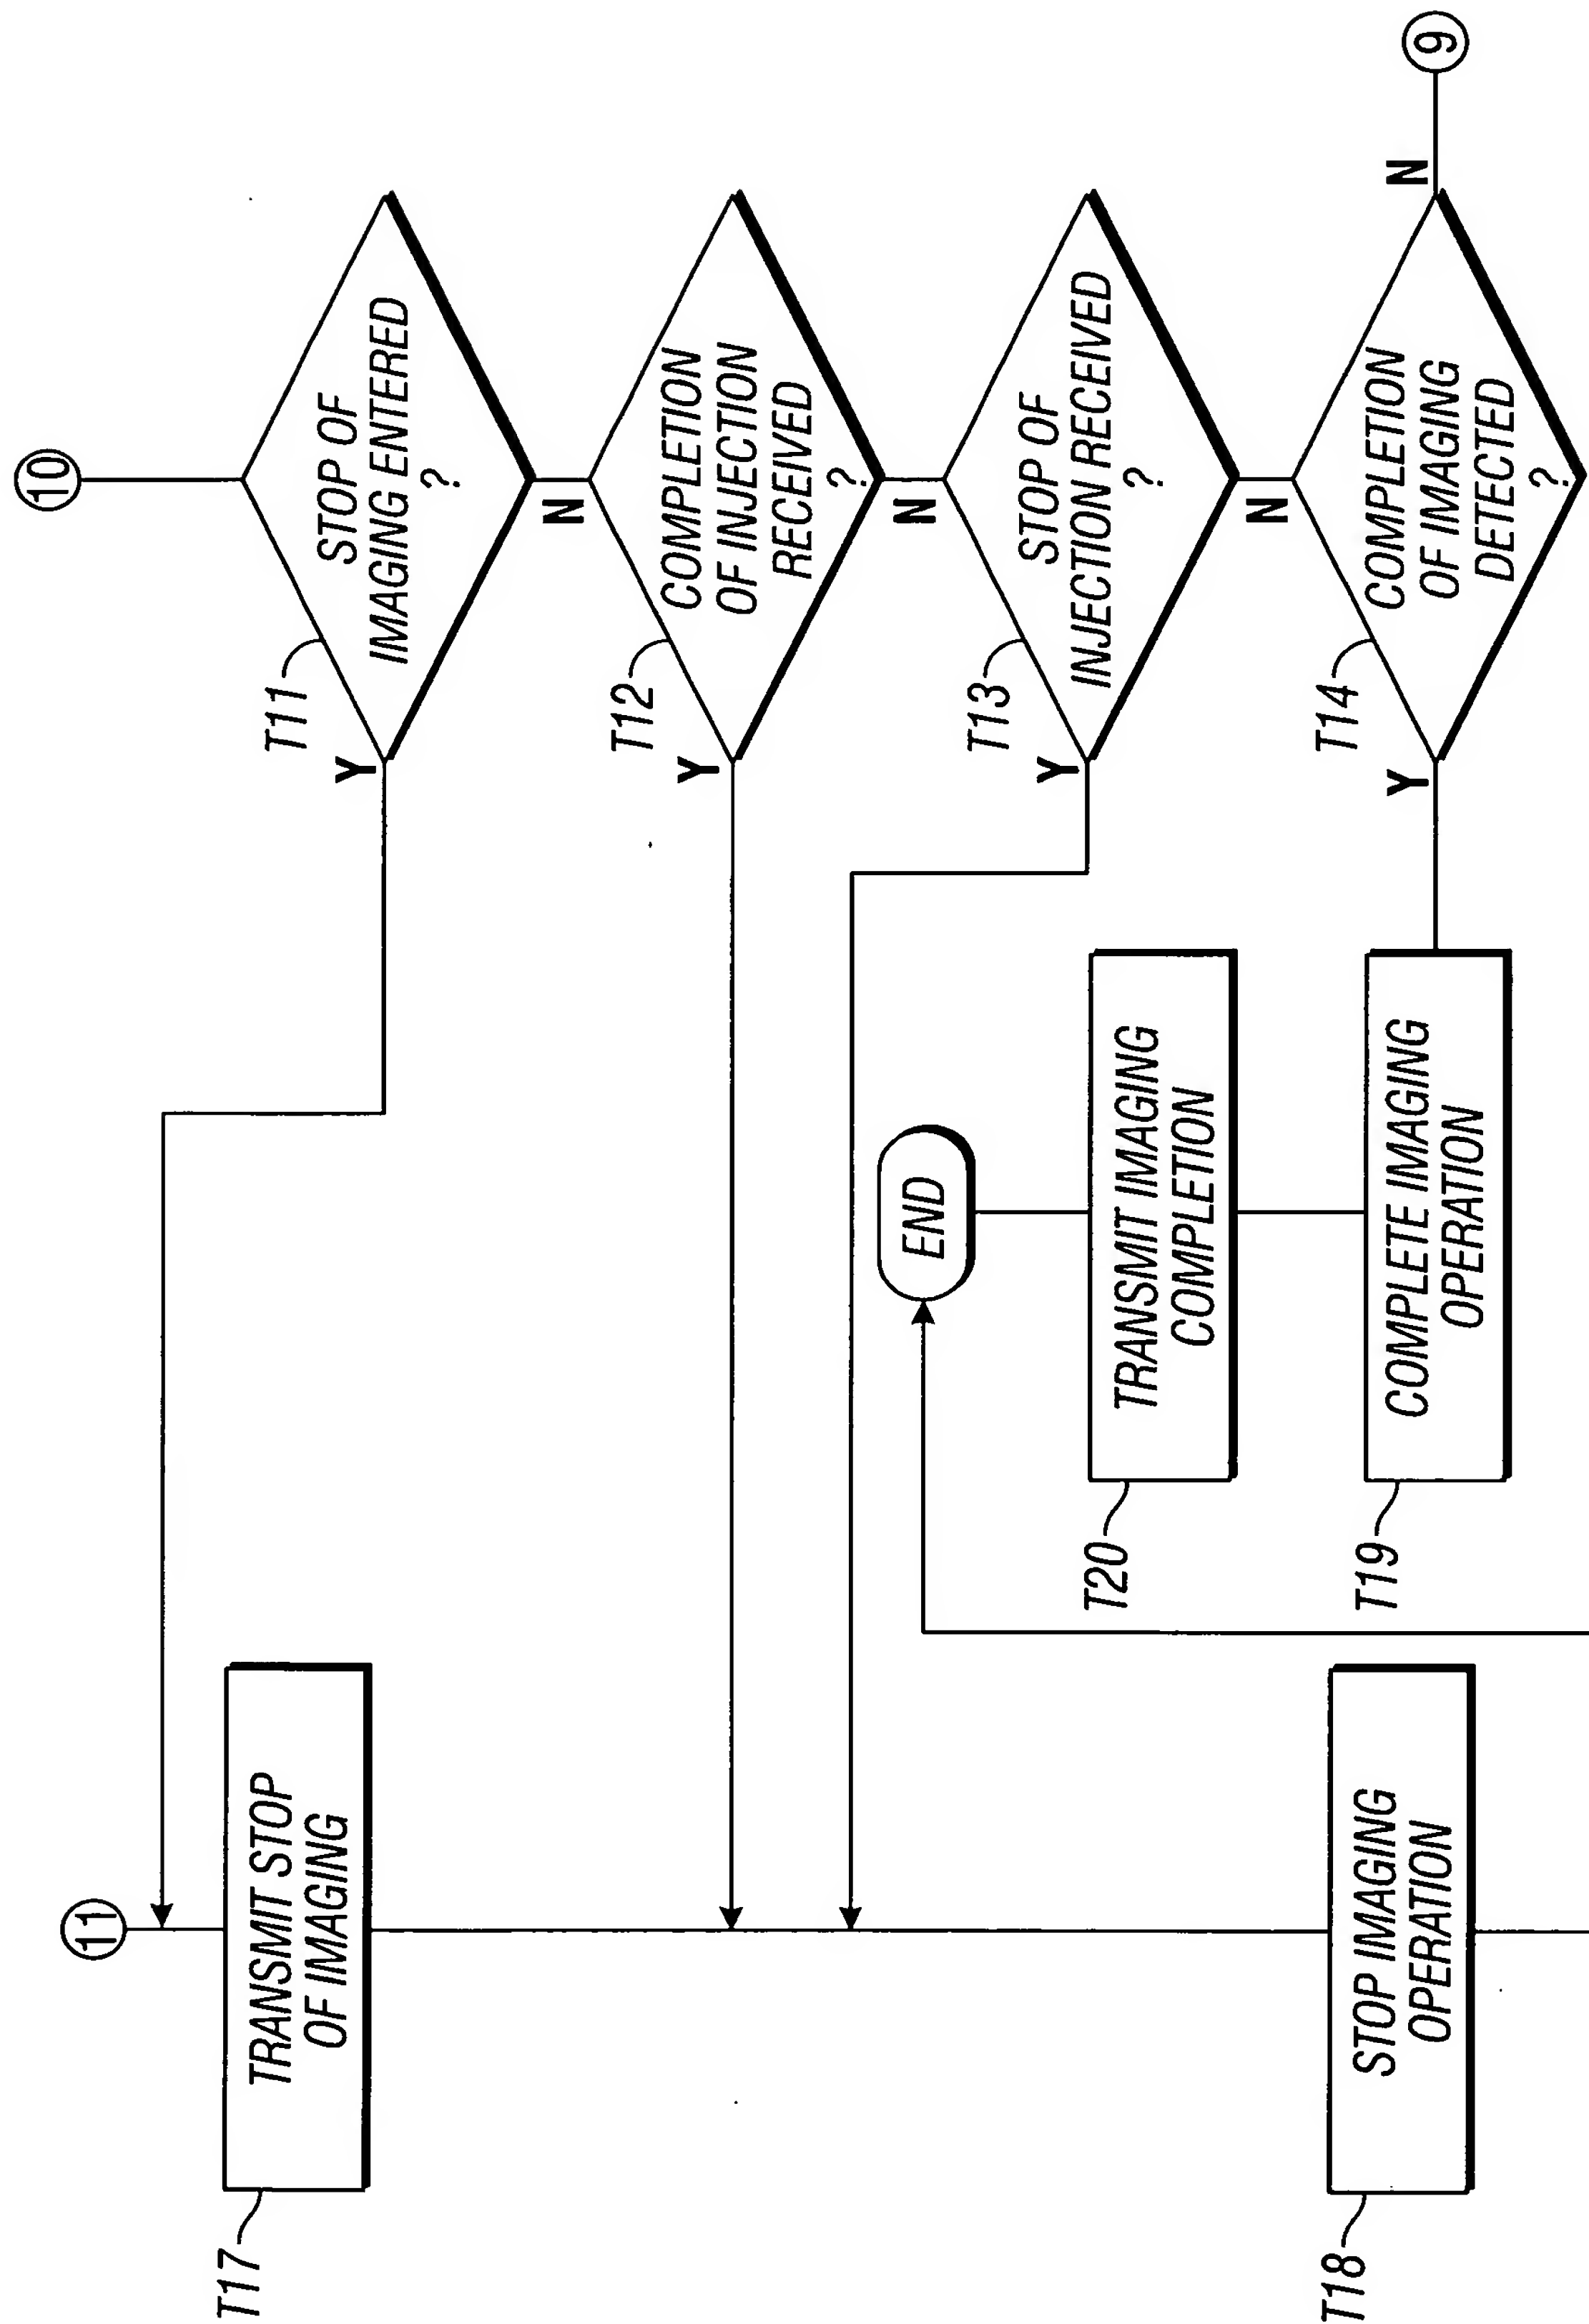


FIG. 16
(Continued)

16/16

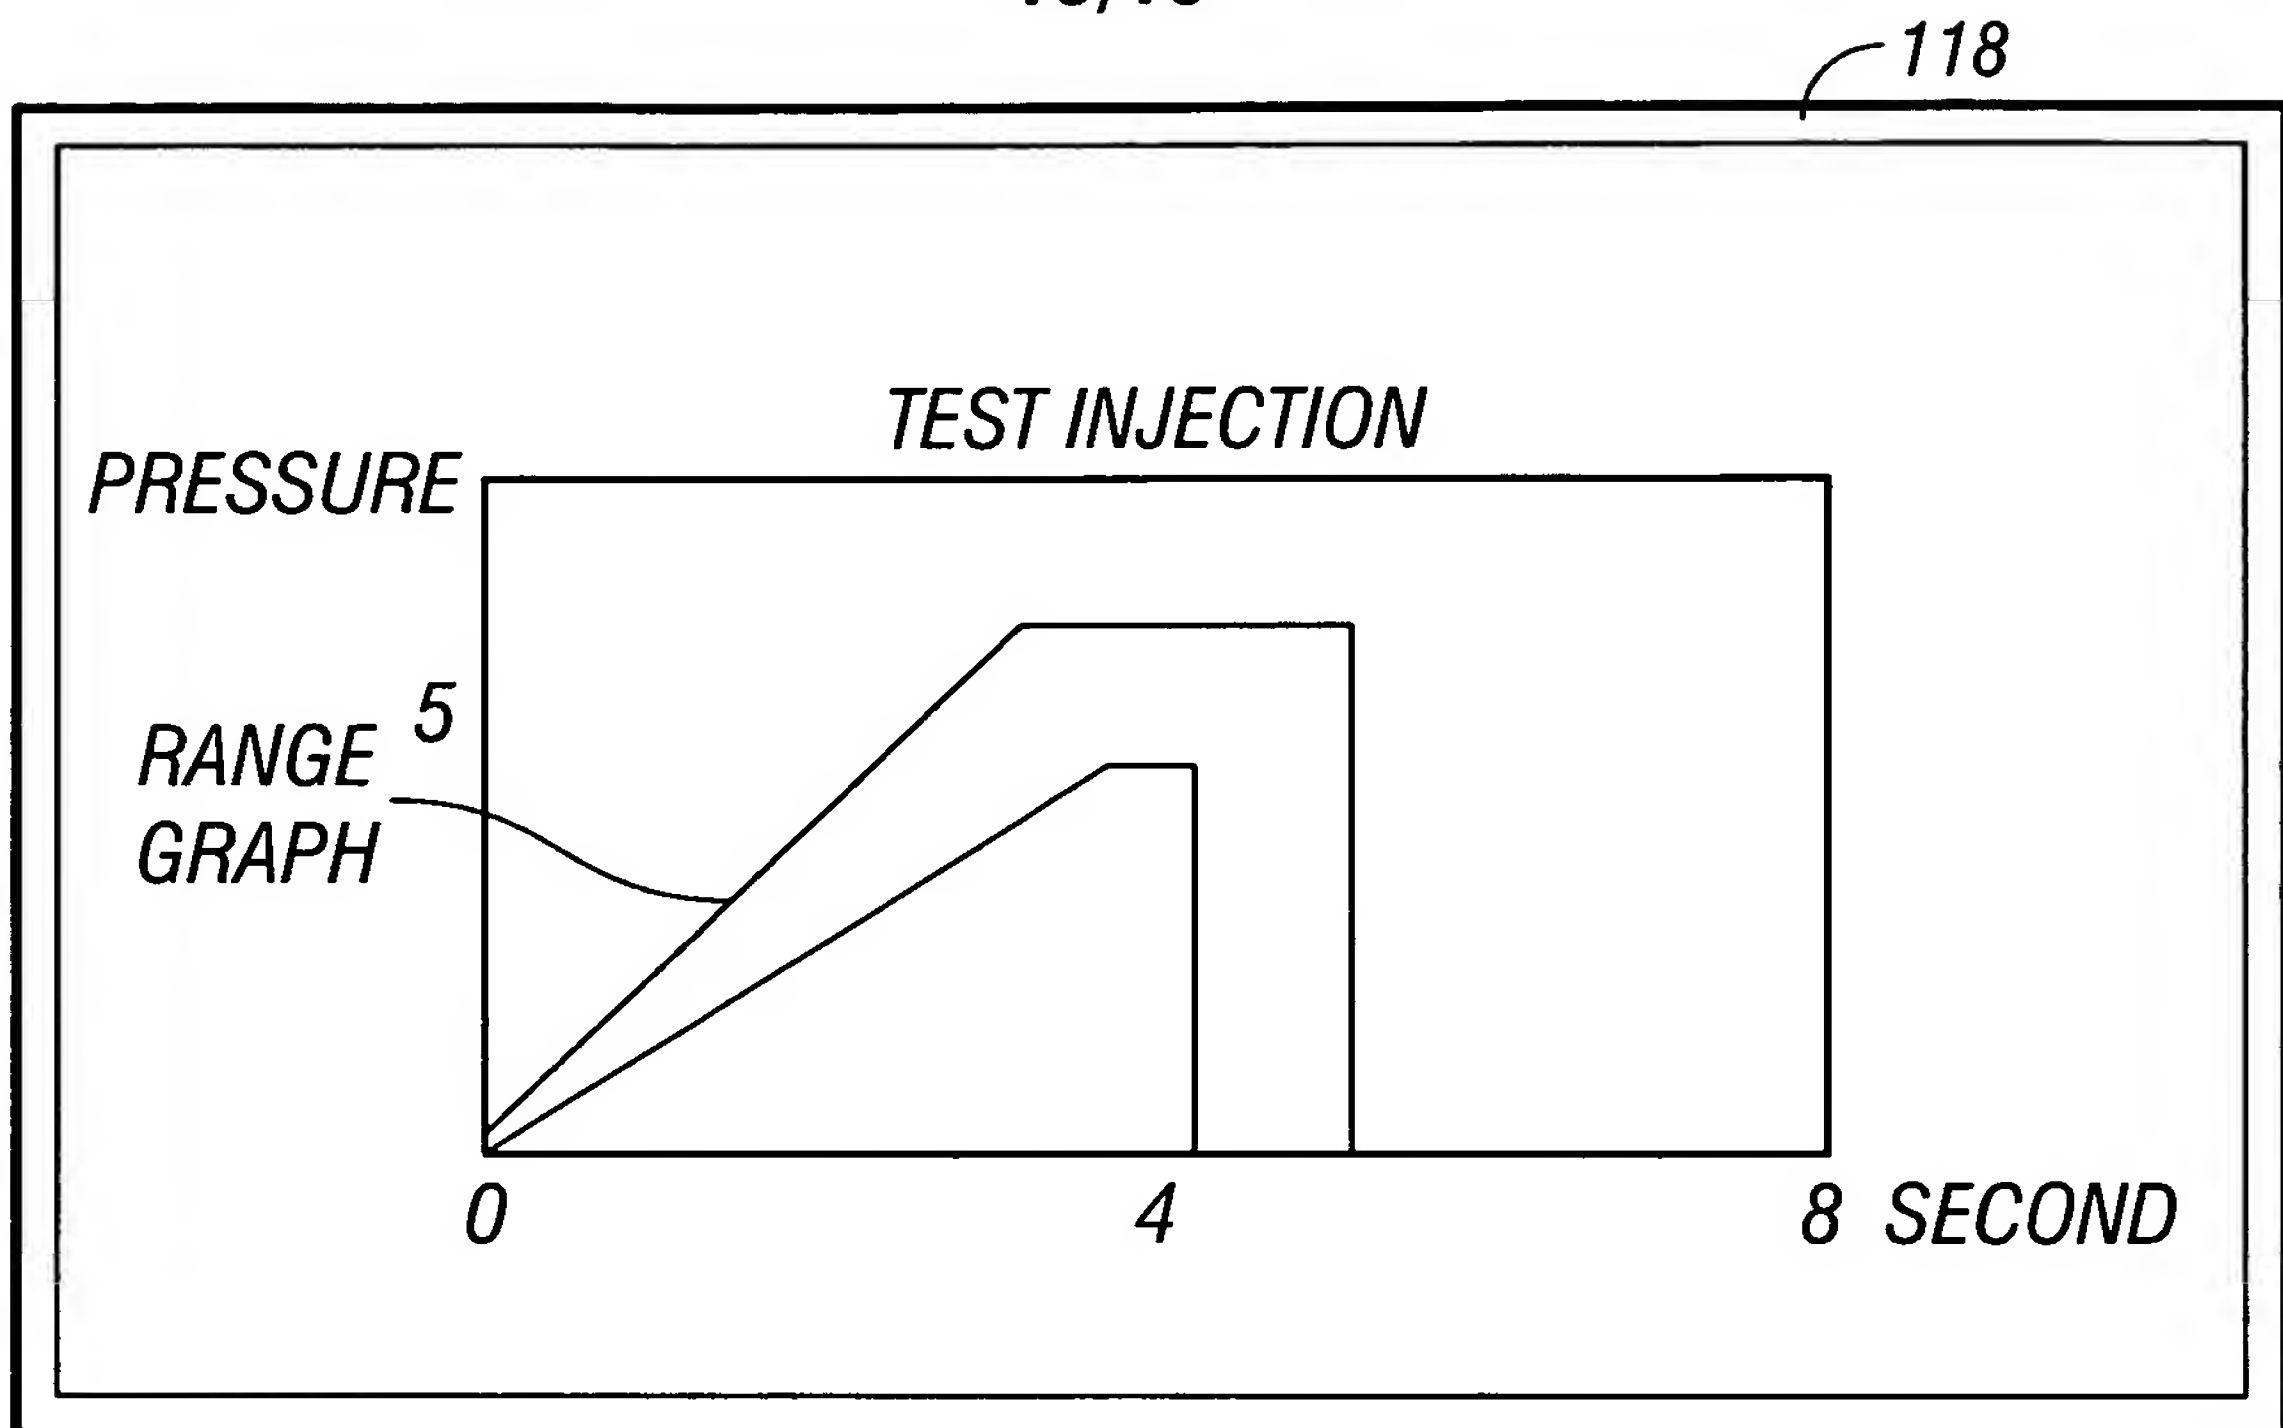


FIG. 17

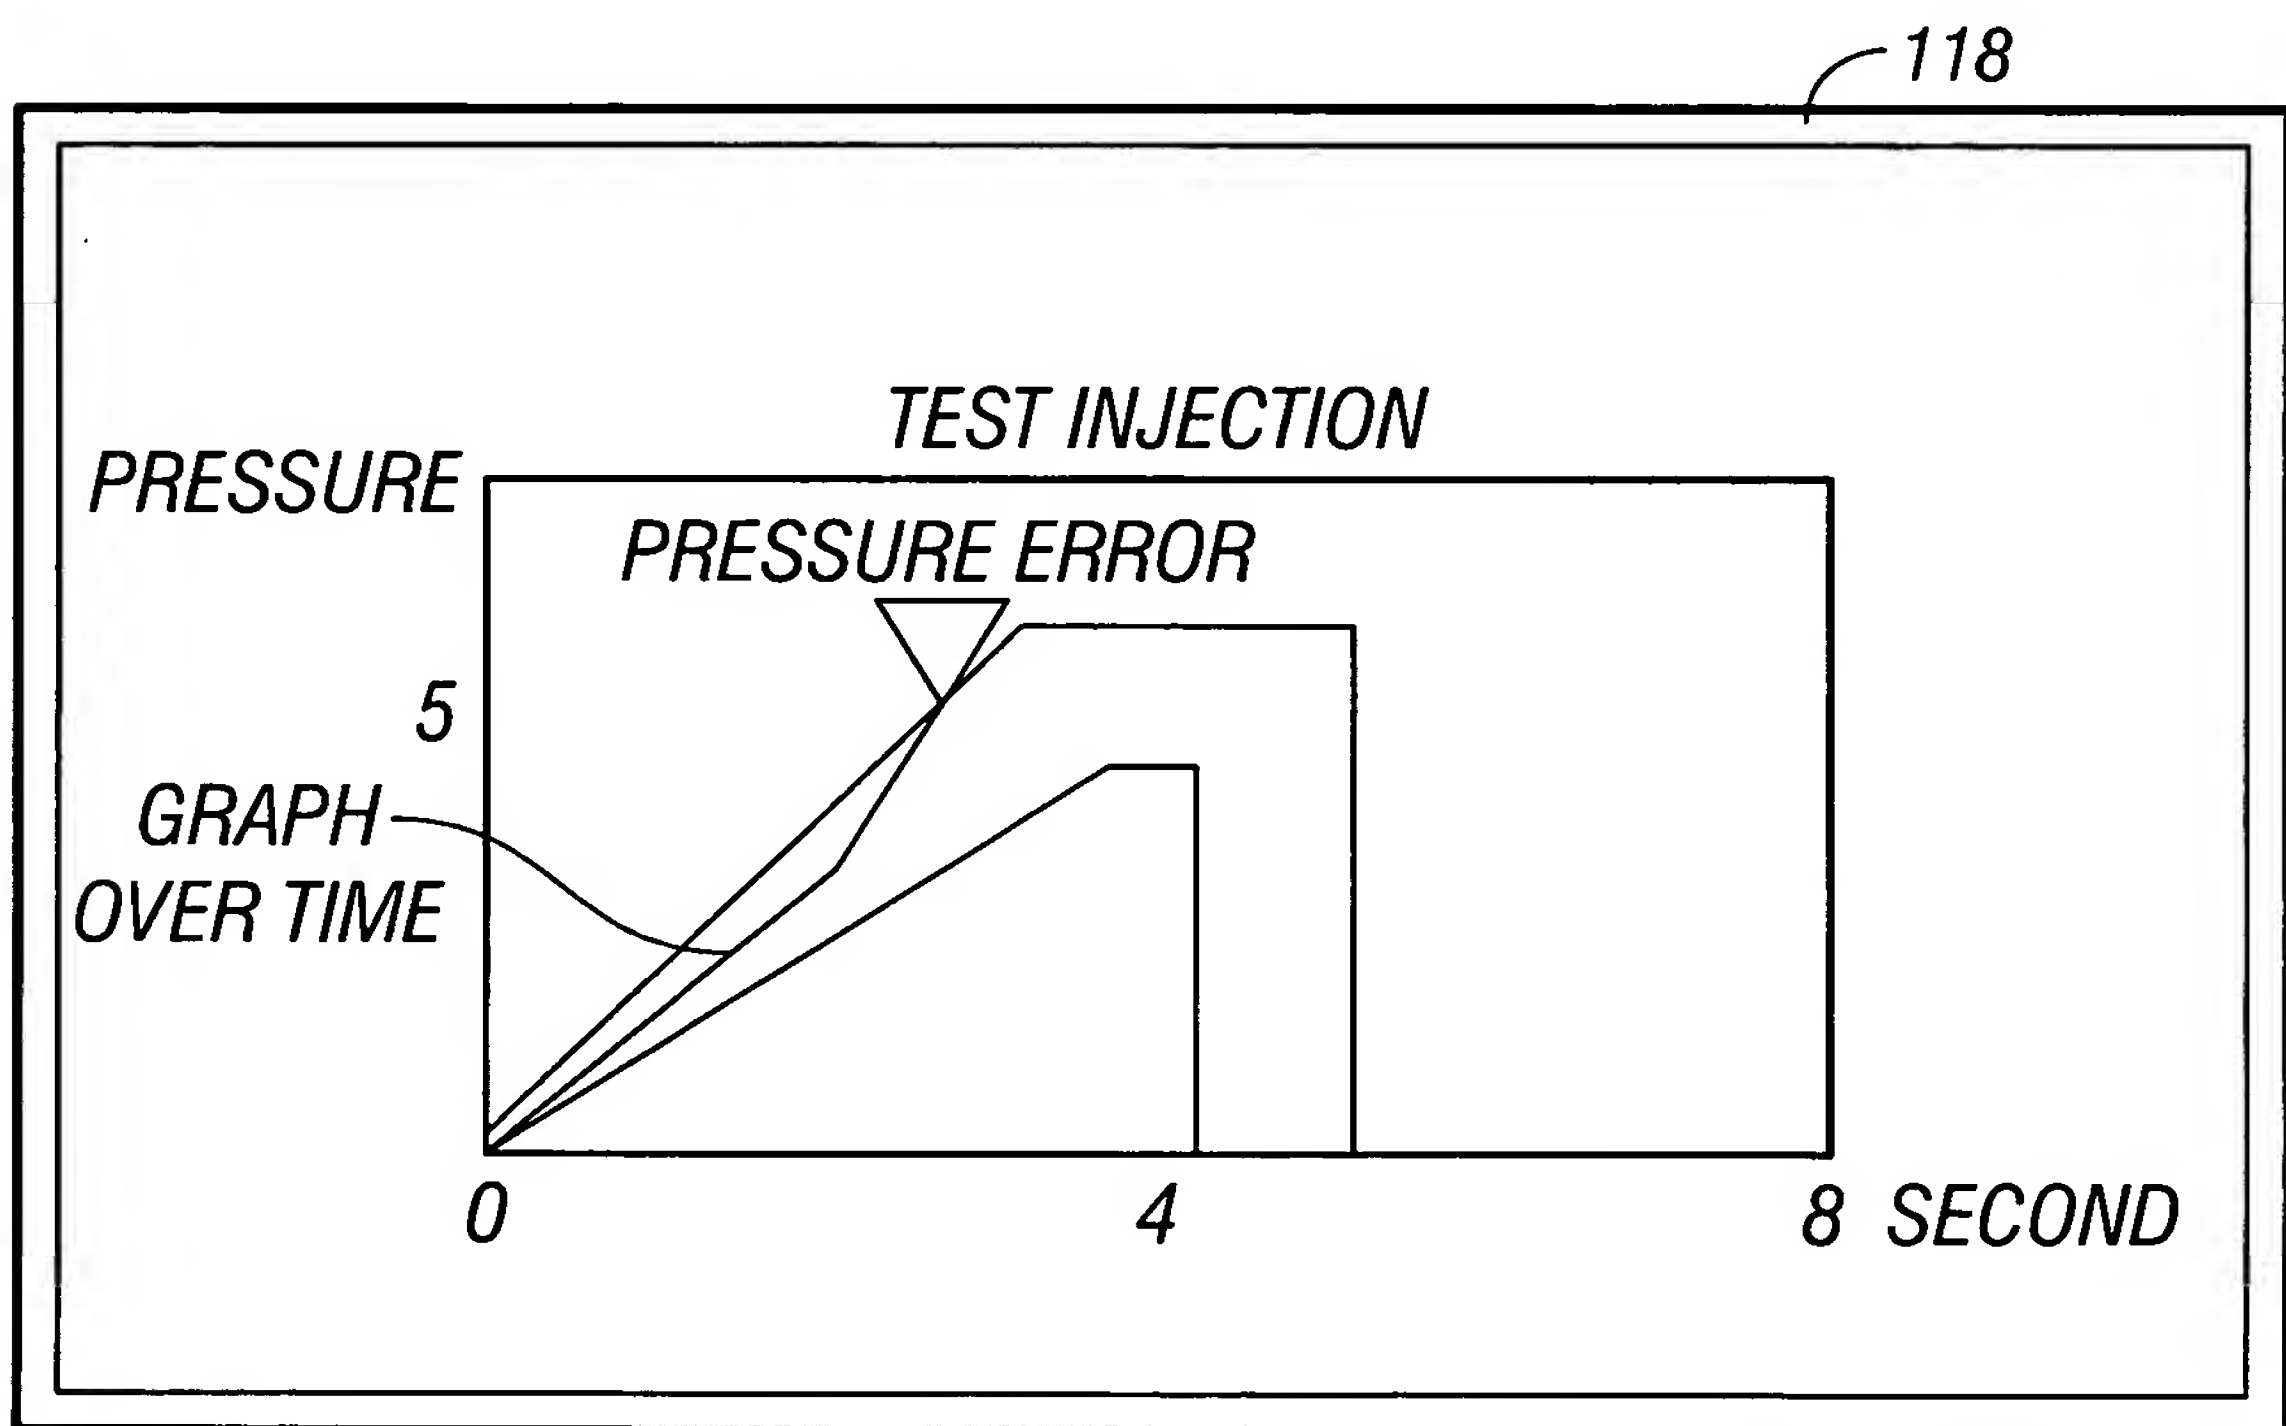


FIG. 18